

## Radioisotopes in action



## Diagnostic application of radioisotopes

### Optimal activity for diagnostic procedure

Maximize the information

Minimize the risk

$$\Lambda \sim 100 \text{ MBq}$$

### Types of images

Static picture – spatial distribution of isotope / activity  
at a certain time

Dynamic picture – variation of the amount of isotope /  
activity in time

Static and dynamic picture – series of static recordings


#### Emission CT

SPECT (Single Photon Emission Computed Tomography)


PET (Positron Emission Tomography)

### Types of images

Static picture – spatial distribution of isotope / activity  
at a certain time



thyroid glands




kidneys



Isotope accumulation in

## Types of images

Dynamic picture – variation of the amount of isotope / activity in time

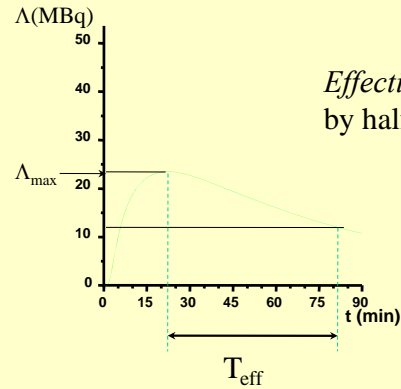

*Effective half-life* – activity decreases by half in the target organ

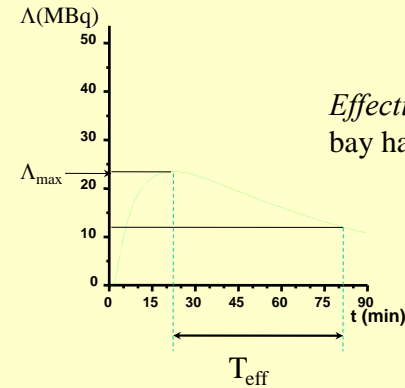

*Effective half-life* – activity decreases by half in the target organ


$$\Lambda = \Lambda_0 e^{-(\lambda_{phys} + \lambda_{biol})t}$$

$$\lambda_{effective} = \lambda_{phys} + \lambda_{biol}$$

$$\frac{1}{T_{eff}} = \frac{1}{T_{phys}} + \frac{1}{T_{biol}}$$

The final fate of the radiotracer depends on how the addressed organ deals with the molecule, whether it is absorbed, broken down by intracellular chemical processes or whether it exits from the cells and is removed by kidney or liver processes. These processes determine the **biological half-life**  $T_{biol}$  of the radiopharmaceutical.


example

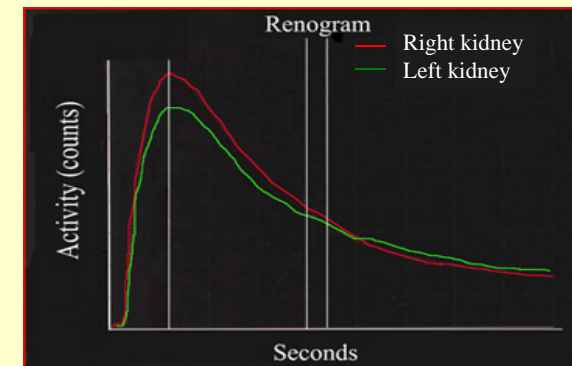


kidney

Isotope accumulation

example

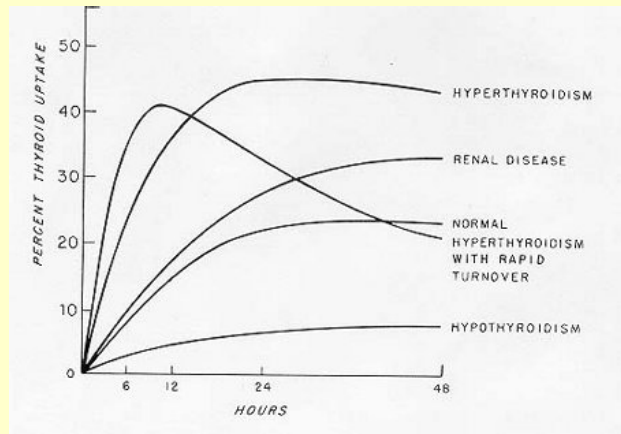

Thyroid glands  
Isotope accumulation

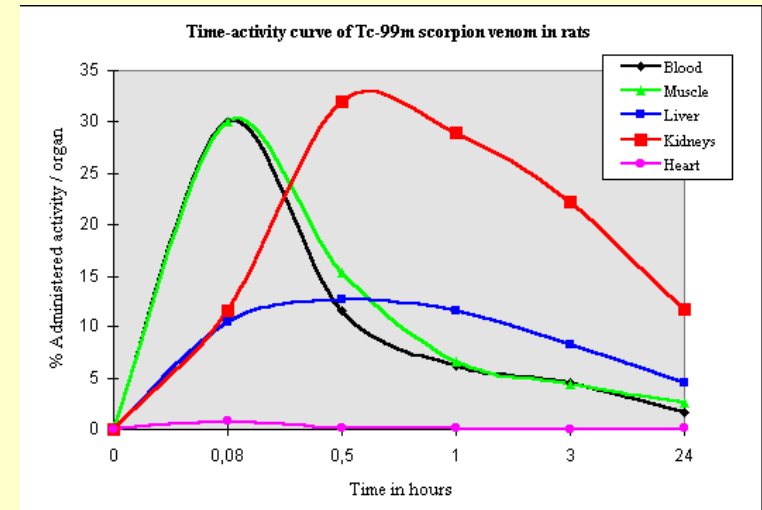

Hal Anger  
1920-2005




Hal Anger and coworkers  
1952





Gamma camera

Photomultiplier tubes  
Scintillation crystal  
Collimator

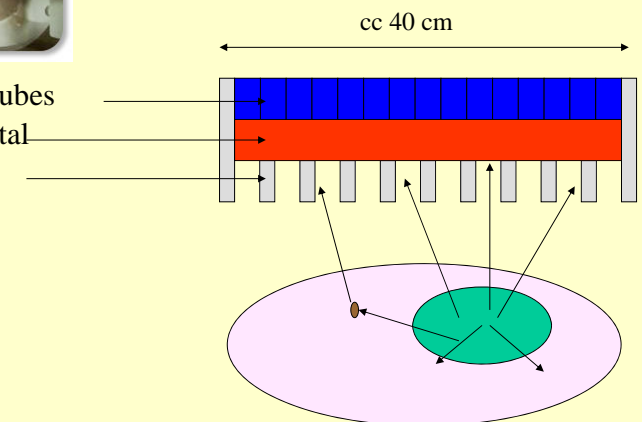

A radioactive source emits gamma ray photons in all directions.

collimator

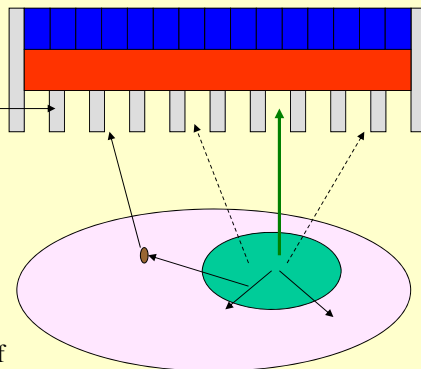


Collimators are composed of thousands of precisely aligned channels made of lead.

The collimator conveys only those photons traveling directly along the long axis of each hole.

Photons emitted in other directions are absorbed by the septa between the holes.


Size and geometry of holes are essential for the resolution.



## Scintillation crystal



NaI(Tl)

Sufficient detection efficiency  
photons of 150 keV  $\mu \sim 2.2 \text{ 1/cm}$   
10 mm thickness  $\sim 90\%$  attenuation  
Proper wavelength – 415 nm – for PM photocathode

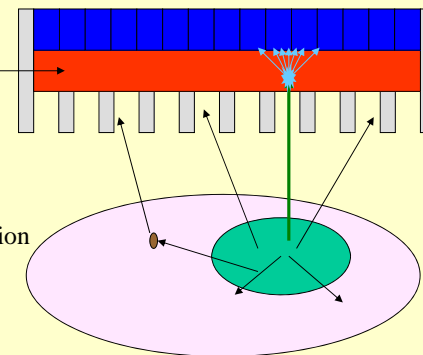


Problems:

fragile  
temperature sensitive  
hygroscopic



## Photomultiplier tubes

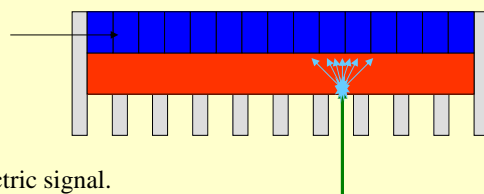


Transformation of light pulses to electric signal.


Typically 37-91 tubes, 5.1-7.6 cm diameter each

Amplitude of electric pulses varies in a wide range, because

- absorption of one  $\gamma$ -photon induces electric signals in more than one tubes.
- attenuation mechanism can be photoeffect and Compton-scatter.

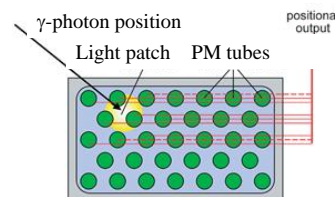


Pulse amplitude spectrum – Amplitude of an electric pulse generated by a  $\gamma$ -photon absorption in photoeffect is proportion to the photon energy.

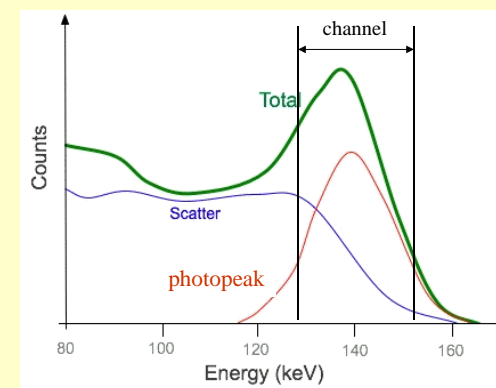






These electric pulses can be distinguished by discrimination (DD).

## Gamma camera

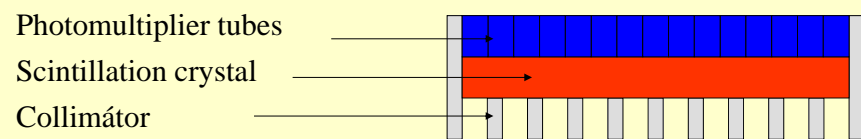


Identification of source position is facilitated by  
the collimator  
the PM tubes  
the discrimination.

Pertechnetate (intravenous 80 MBq) distribution in thyroid glands




Liver lesion nodules

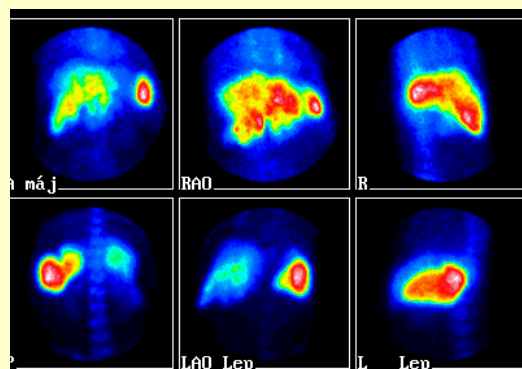

$^{99m}\text{Tc}$ -fyton

## Bone scintigraphy

$^{99m}\text{Tc}$ -MDP: 600 MBq

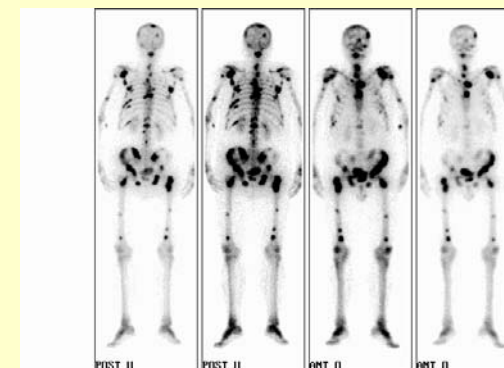

Gamma camera – space and time distribution can be recorded

static and dynamic pictures can be reconstructed



Camera parameters:

spatial resolution

energy resolution

efficiency of detection


## Gamma camera image: summation image

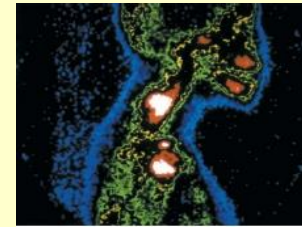

For depth resolution: tomographic device is necessary

## SPECT

Single Photon Emission Computed  
Tomography

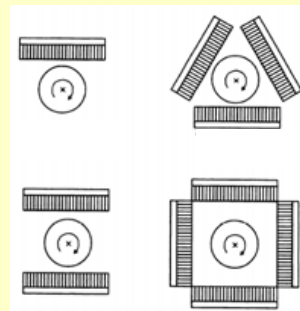

Various camera arrangements

## SPECT


Tomographic application of  $\gamma$ -cameras – data collection in  $360^\circ$ .

Cross-sectional image can be reconstructed.



Measurement from a series of projections.

Computer directs the movement of the detector, stores the data,  
reconstruct the cross-sectional image

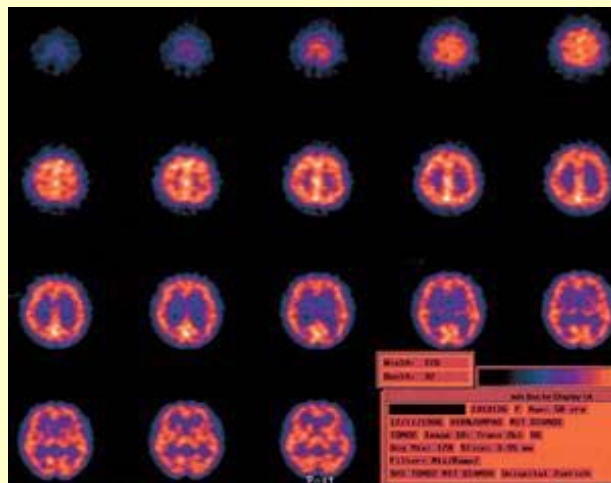


$^{99m}\text{Tc}$ - HMPAO

## Positron Emission Tomography

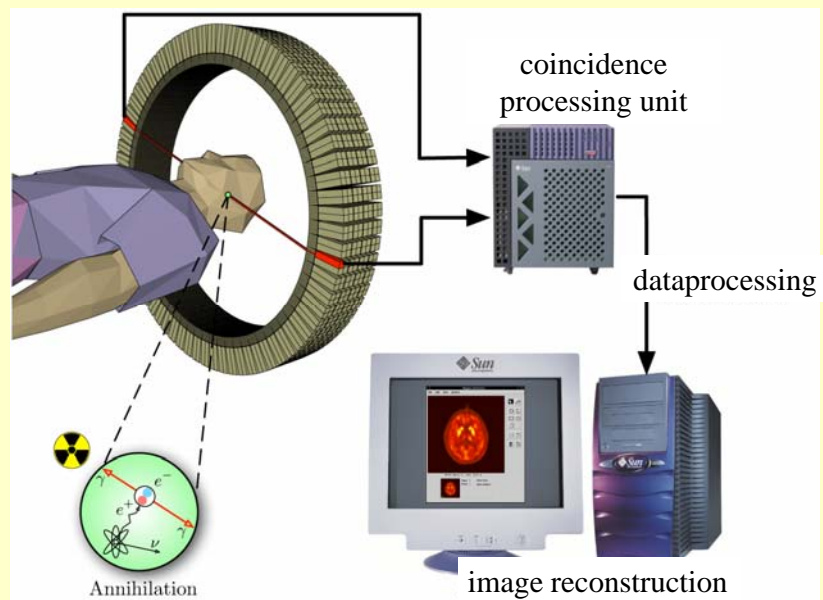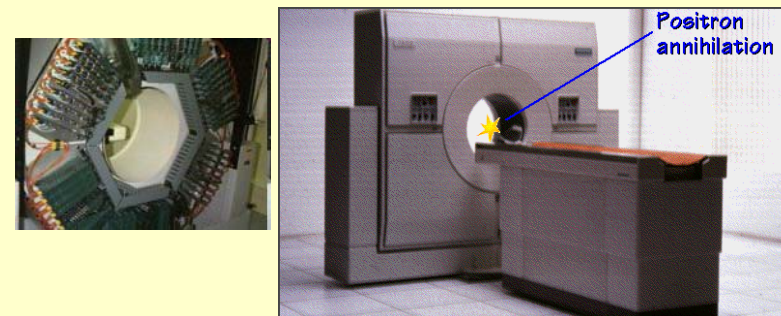

coincidence processing

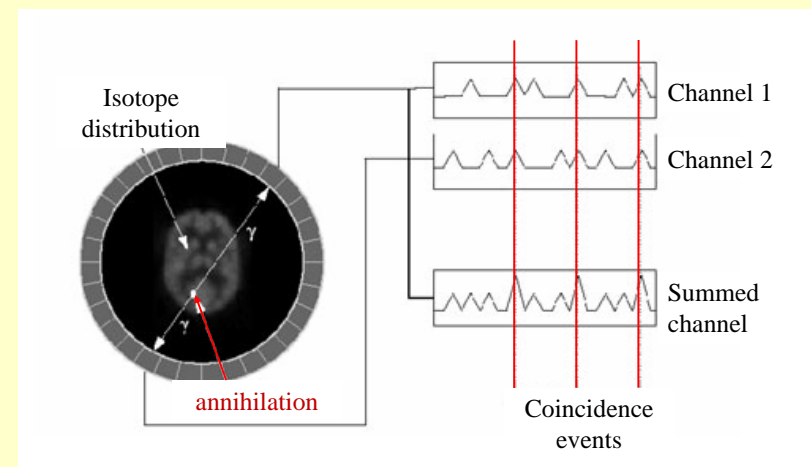

The most frequently used radionuclides in PET are radioisotopes of structural elements of natural organic molecules.



Isotope	$\beta^+$ energy (MeV)	$\beta^+$ range (mm)	1/2-life	Applications
$^{11}\text{C}$	0.96	1.1	20.3 min	receptor studies
$^{15}\text{O}$	1.70	1.5	2.03 min	stroke/activation
$^{18}\text{F}$	0.64	1.0	109.8 min	oncology/neurology
$^{124}\text{I}$	2.1350/1.5323	1.7/1.4	4.5 days	oncology

Isotope manufacturing nearby the site of application (see half-lives).



## PET/CT

Combination of structural and functional imaging

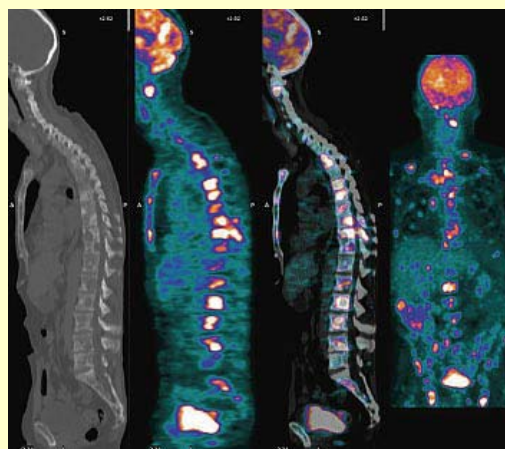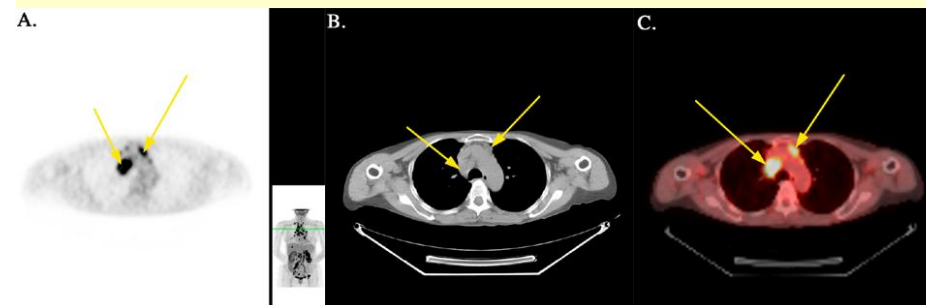


CT

PET


PET/CT

PET


## Activity of brain areas

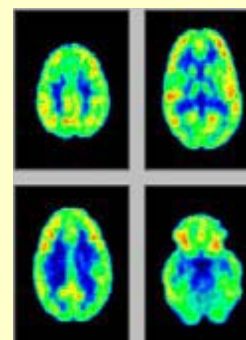

In rest

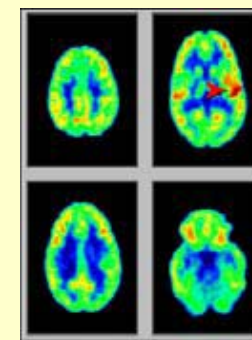

hearing

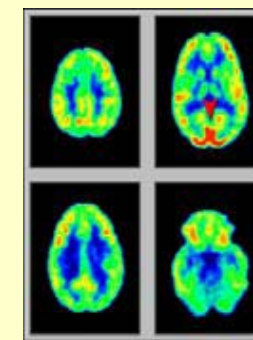

vision



*Damjanovich, Fidy, Szöllősi: Medical biophysics*

II. 3.2.3

3.2.4

3.2.5

VIII. 3.2

VIII. 4.4

IX.3