

MEDICAL BIOPHYSICS II

MEDICAL BIOPHYSICS II

- X-ray - generation and properties
- X-ray - diagnostic foundations
- Medical use of electronics
- Thermodynamics - equilibrium, change, laws
- Diffusion, Brown-motion, Osmosis
- Flow of fluids and gases. Hemodynamics
- Bioelectric phenomena
- Sound, ultrasound
- Biophysics of sensory organs. Vision and hearing
- Building blocks of life: water, macromolecules, supramolecular systems
- Methods of investigating biomolecular structure and dynamics. MRI
- Molecular mechanisms of biomolecular motion. Biomechanics, biomolecular and tissue elasticity
- Respiratory and cardiac biophysics. Physical examination

X-RAY

GENERATION, SPECTRAL FEATURES
INTERACTION WITH MATTER

X-RAY




Wilhelm Konrad
Röntgen
(1845-1923)
Nobel prize, 1901



Hand mit Ringen (Hand with Ring): print of Wilhelm Röntgen's first "medical" X-ray, of his wife's hand, taken on 22 December 1895 and presented to Professor Ludwig Zehnder of the Physik Institut, University of Freiburg, on 1 January 1896. The dark oval on the third finger is a shadow produced by her ring.

PAPER FUNNEL RADIOSCOPE

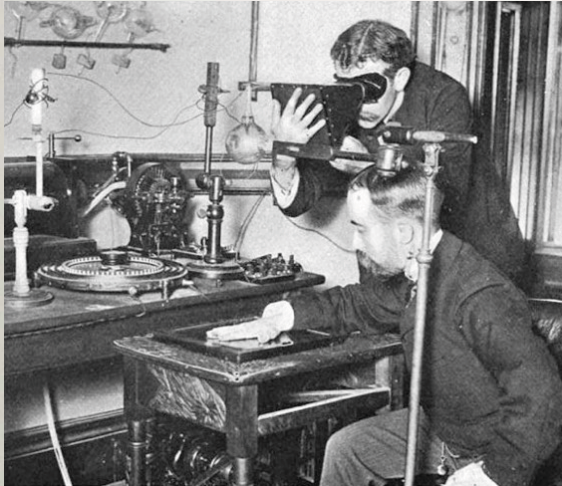

Late 1890s



I. World war

MEDICAL DIAGNOSTICS



1940



1950



today

SHOE-FITTING FLUOROSCOPE (1930-50)



CERTIFICATE

SHOE-FITTING TEST DATA FOR _____

1. ANKLE ROLL GOOD ☐ FAIR ☐ POOR ☐

2. WEIGHT DISTRIBUTION

3. X-RAY FITTING TEST

LEFT RIGHT LEFT RIGHT

40% 60% 30% 70%

RIGHT WAY WRONG WAY RIGHT WAY WRONG WAY

GOOD FAIR POOR

Wavelength is about 3 football fields long.

Wavelength is about 3 m or 10 feet long.


Wavelength is about 3 cm or 1 inch long.

Wavelengths 400-700 nm

Wavelength about 30 x diameter of hydrogen atom

This scientific way of approaching the problem of poorly-fitted shoes eliminates guesswork. Now you can see for yourself!

X-RAYS ARE ELECTROMAGNETIC WAVES

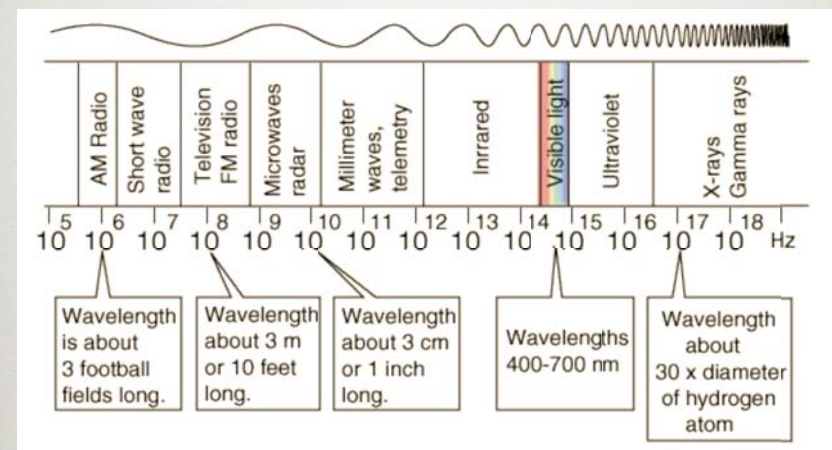


Wavelength 10 - 0.01 nm. Frequency 30×10^{15} - 30×10^{18} Hz. Energy 120 eV - 120 keV.

X-RAYS

- Generation of X-rays
- X-ray spectrum
- Interaction with matter 1: diffraction
- Interaction with matter 2: absorption
- X-ray absorption mechanisms:
Photoelectric effect
Compton scatter
Pair production

GENERATION OF X-RAY (NON-CONVENTIONAL)

Triboluminescence: light emission evoked by scratching or rubbing. Francis Bacon, 1605.

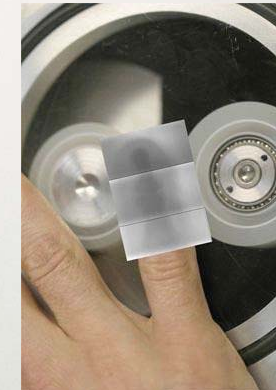

Peeling away sticky tape emits light...

...and X-rays. (Nature News, October 2008)

GENERATION OF X-RAY: IN CATHODE RAY TUBE



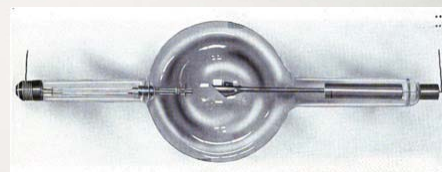


Photo of a Coolidge x-ray tube, from the early 1900s. The heated cathode is on the left, the anode target is on the right. The x-rays are emitted in a downward direction.

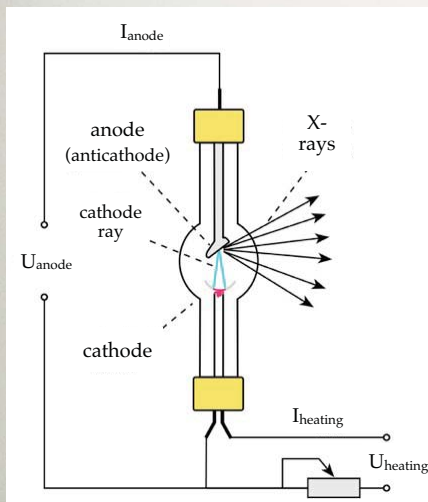


Rotating anode X-ray tube

“BREMSSTRAHLUNG”

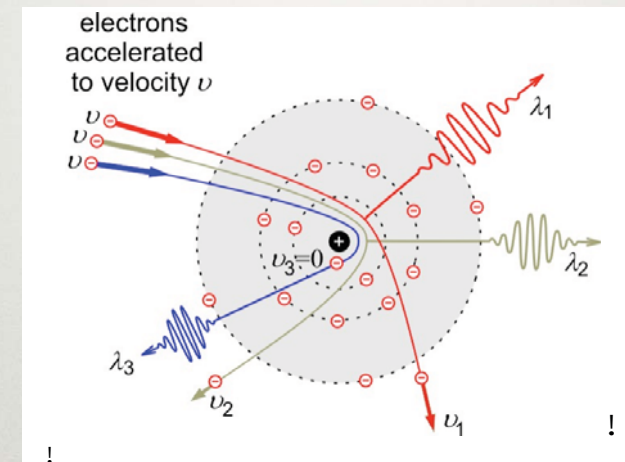


Electrons decelerate, thereby lose their kinetic energy, when interacting with the atoms of the anode (“braking radiation”).

SPECTRUM OF BREMSSTRAHLUNG

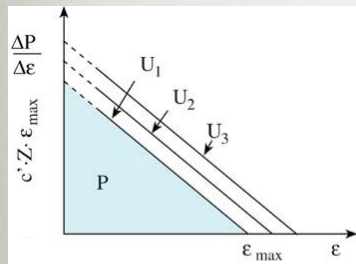

Continuous spectrum

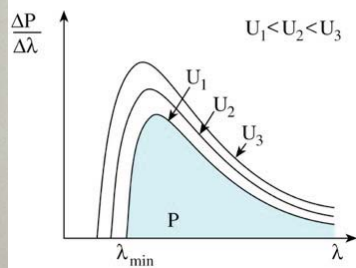

$$eU_{anode} = \epsilon_{max} = hf_{max}$$

Maximal photon energy (ϵ_{max})

h = Planck's constant; c = speed of light; e = charge of electron; eU_{anode} = work of acceleration

$$\lambda_{min} = \frac{hc}{e} \cdot \frac{1}{U_{anode}}$$

Limiting wavelength (λ_{min})
(Duane-Hunt Law)

$$\frac{\Delta P}{\Delta \epsilon} = c' \cdot Z \cdot (\epsilon_{max} - \epsilon)$$

Energy spectrum
(energy dependence of power)

$$P_{tot} = \frac{1}{2} c' \cdot Z \cdot \epsilon_{max}^2 = c \cdot Z \cdot U_{anode}^2 \cdot e^2$$

Total power
(based on area of triangle)


$$P_{tot} = C_{Rtg} \cdot I_{anode} \cdot U_{anode}^2 \cdot Z$$

Total power


$$\eta = \frac{P_{tot}}{P_{in}} = \frac{C_{Rtg} \cdot I_{anode} \cdot U_{anode}^2 \cdot Z}{I_{anode} \cdot U_{anode}} = C_{Rtg} \cdot U_{anode} \cdot Z$$

Efficiency <1%

CHARACTERISTIC X-RAY

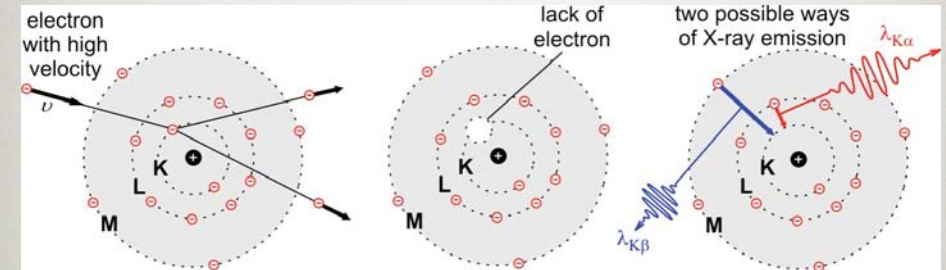


Knocked-out inner-shell electron is replaced by one on a higher-energy shell

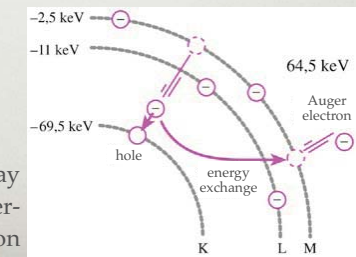

Energy of electron transition may be used for the escape of an outer-shell electron: Auger electron


SPECTRUM OF CHARACTERISTIC X-RAY

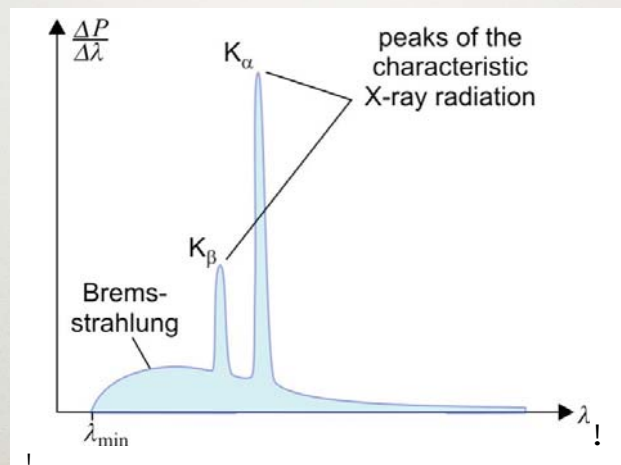


Line spectrum

X-RAY SPECTRUM CHARACTERIZES THE ELEMENT

Because inner-shell electrons participate in characteristic X-radiation, only the atomic (and not the molecular) properties are revealed

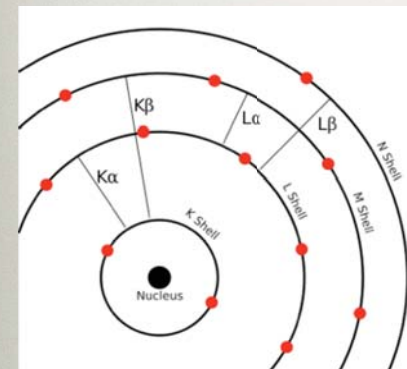


Electronic transitions in a calcium atom.

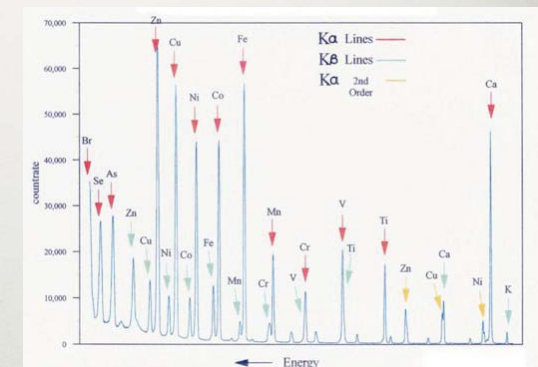


Energy dispersive X-ray fluorescence spectrum.

DETECTION OF CHARACTERISTIC X-RAY



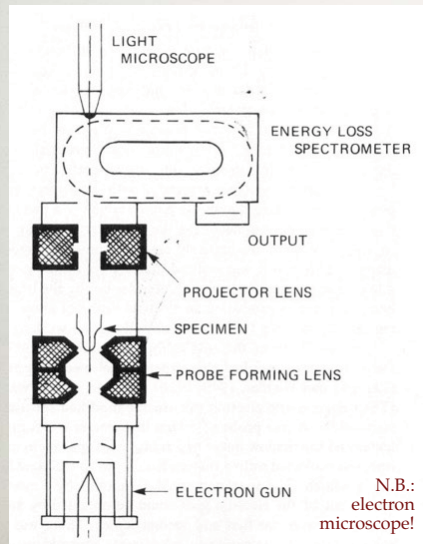


Electron probe microanalyzer

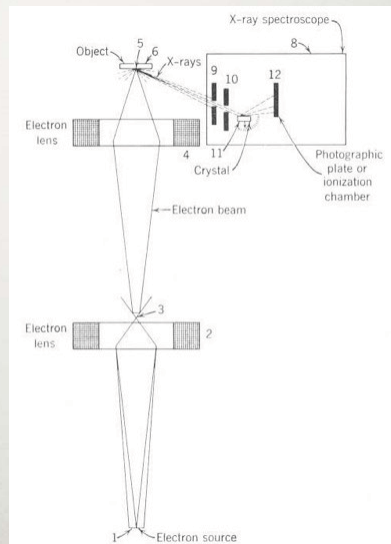


X-ray spectroscopy

X-RAY DIFFRACTION

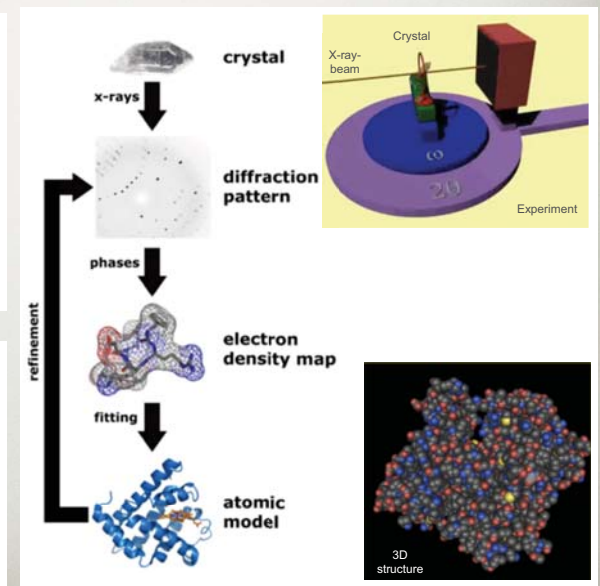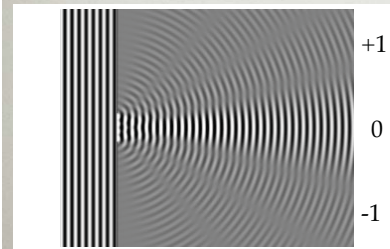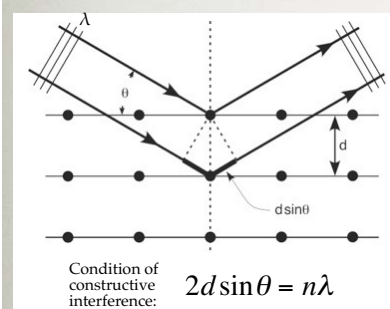

X-RAY ABSORPTION

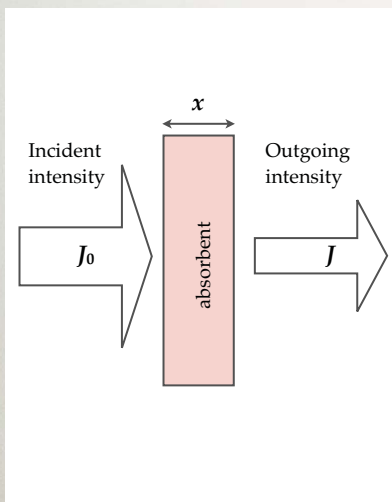


Exponential attenuation principle

$$J = J_0 e^{-\mu x}$$

$$\mu = \mu_m \rho$$

μ =attenuation coefficient
 μ_m =mass attenuation coefficient (cm^2/g)
 ρ =density (g/cm^3)

X-RAY PHOTOEFFECT

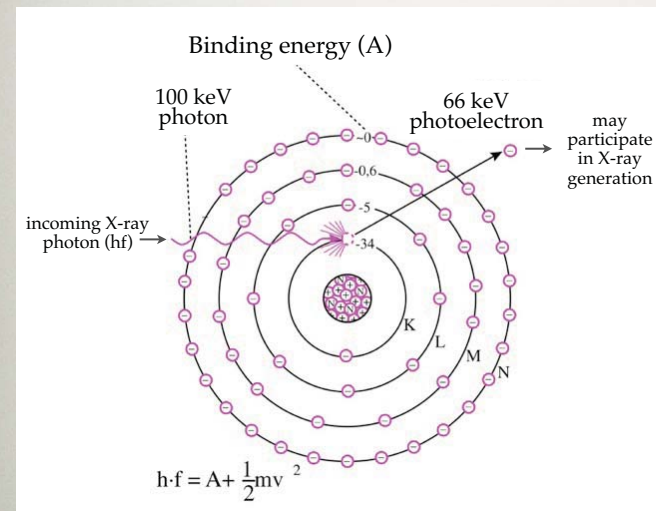


Main effect in diagnostic X-ray!

Photoeffect attenuation coefficient:

$$\tau = \tau_m \rho$$

PHOTOEFFECT ATTENUATION DEPENDS STRONGLY ON ATOMIC NUMBER

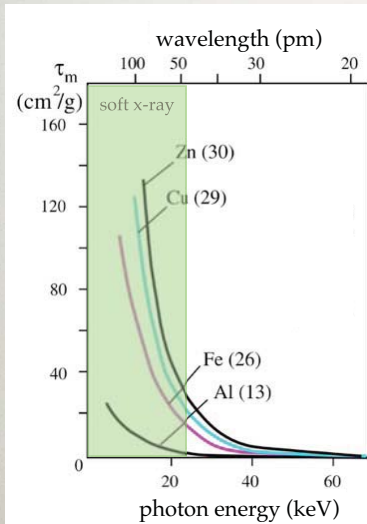

$$\tau_m = \text{const} \cdot \frac{Z^3}{\varepsilon^3} = C \cdot \lambda^3 \cdot Z^3$$


For multi-component system:
"effective atomic number" (Z_{eff})

$$Z_{\text{eff}} = \sqrt[n]{\sum_{i=1}^n w_i Z_i^3}$$

ε =photon energy
 Z =atomic number
 w =mole fraction
 n =number of components


Material	Z_{eff}
Air	7.3
Water	7.7
Soft tissue	7.4
Bone	13.8

COMPTON SCATTER




Arthur Holly
Compton
(1892-1962)

$$hf = A + hf_{\text{scatt}} + E_{\text{kin}}$$

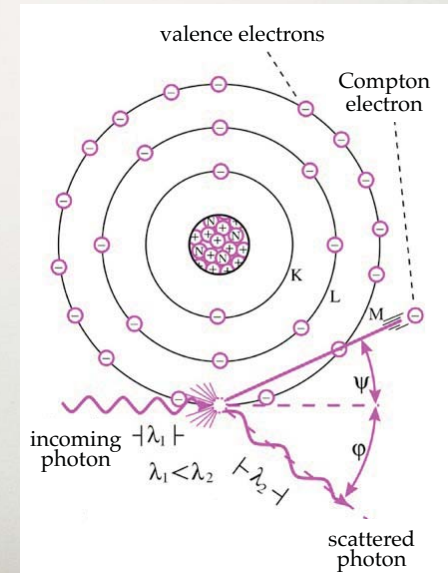

PAIR PRODUCTION

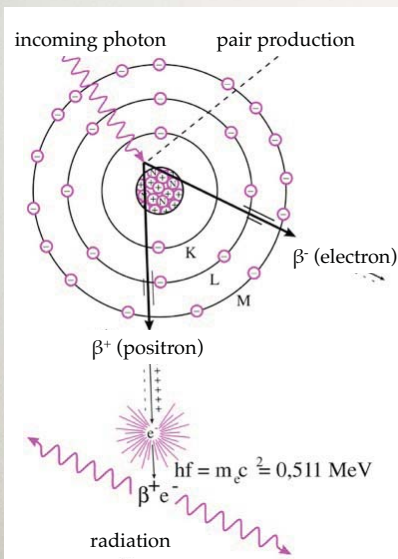

(relevant only in therapeutic x-ray)

Energy balance:



$$hf = 2m_e c^2 + 2E_{\text{kin}}$$

m_e =mass of electron
 c =speed of light

Pair production relevant in high-energy X-ray photons, γ -radiation.

ATTENUATION MECHANISMS

Dependence on photon energy and material

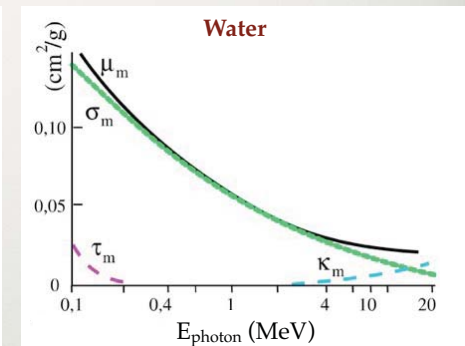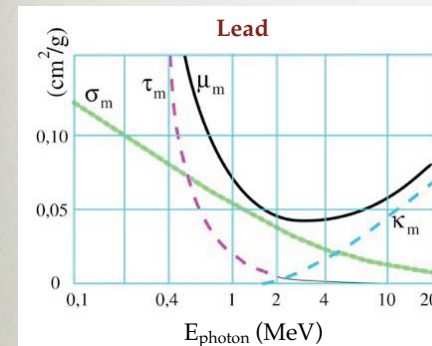

$$\mu = \tau + \sigma + \kappa$$

μ_m =mass attenuation coefficient
 σ_m =Compton effect mass attenuation coefficient

τ_m =photoeffect mass attenuation coefficient
 κ_m =pair production mass attenuation coefficient

SUMMARY OF ATTENUATION MECHANISMS


Mechanism	Variation of μ_m with E	Variation of μ_m with Z	Energy range in tissue
Rayleigh	$\sim 1 / E$	$\sim Z^2$	1 - 30 keV
photoelectric	$\sim 1 / E^3$	$\sim Z^3$	10 - 100 keV
Compton	falls gradually with E	independent $\sim Z$	0.5 - 5 MeV
pair production	risks slowly with E	$\sim Z^2$	> 5 MeV

**Main contrast mechanism in diagnostic X-ray:
photoelectric effect ($\sim Z^3$)**


FUTURE TRENDS OF X-RAY APPLICATIONS



Spiral CT

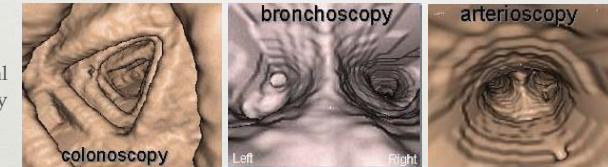

Virtual endoscopy



3D reconstruction



Angiography