

X-ray

Applications

X-ray



Wilhelm Konrad Röntgen
(1845-1923)
Nobel prize in physics, 1901




Hand mit Ringen (Hand with Ring): print
of Wilhelm Röntgen's first "medical" X-
ray, of Anna Bertha Ludwig

X-ray applications


- Diagnostic imaging
The X-ray image
Improvements of X-ray imaging
CAT scanning
- Absorptiometry
Bone density testing
- Therapy
Generation of high-energy X-ray
Tumor irradiation

X-ray absorption

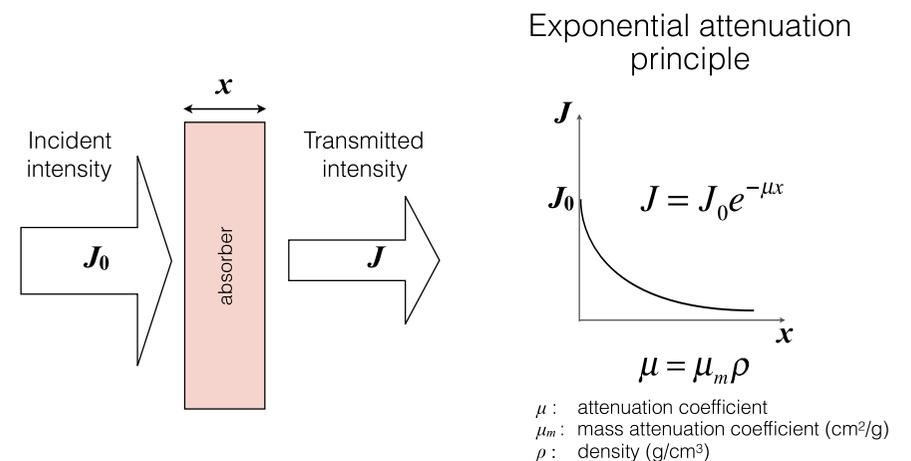

μ_m is the sum of the mass attenuation coefficients
of the different absorption mechanisms.

Attenuation mechanisms

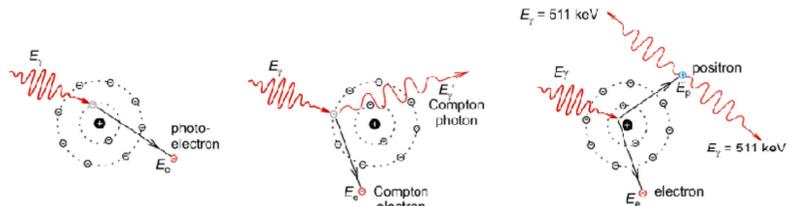

a.) photoeffect

$$E_\gamma = A + E_e$$

$A = \text{work function (escape energy)}$

$$\tau = \tau_m \rho$$

$\tau_m, \sigma_m, \kappa_m$: mass attenuation coefficients, ρ : density

b.) Compton scattering

$$E_\gamma = A + E_e + E_\gamma'$$

$$\sigma = \sigma_m \rho$$

c.) pair production, annihilation

$$E_\gamma = 2 m_0 c^2 + E_e + E_p$$

(if $E_\gamma > 1022 \text{ keV}$)

$$\kappa = \kappa_m \rho$$



$$\mu_m = \tau_m + \sigma_m + \kappa_m$$

Mechanism	Photon energy (ϵ) dependence of the mass attenuation coefficient	Atomic number (Z) dependence of the mass attenuation coefficient	Relevant energy range in soft tissue
Photoeffect	$\sim 1 / \epsilon^3$	$\sim Z^3$	10 - 100 keV
Compton scatter	falls gradually with ϵ	$\sim Z/A$ (A : mass number)	0.5 - 5 MeV
Pair production	rises slowly with ϵ	$\sim Z^2$	$> 5 \text{ MeV}$

Diagnostic X-ray:

1. Contrast mechanism between soft tissue and bone: photoeffect ($\sim Z^3$)
2. Contrast mechanism within soft tissue: Compton-scatter ($\sim \rho$)

Principles of X-ray imaging

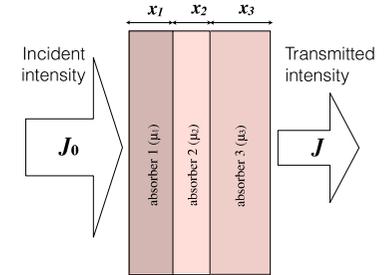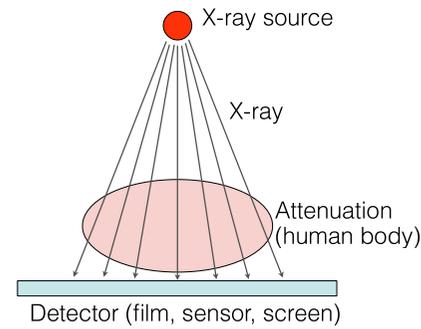

$$J = J_0 e^{-(\mu_1 x_1 + \mu_2 x_2 + \mu_3 x_3 + \dots)}$$

$$\lg \frac{J_0}{J} = (\mu_1 x_1 + \mu_2 x_2 + \mu_3 x_3 + \dots) \cdot \lg e$$


μ_n : n^{th} absorber's attenuation coefficient
 x_n : n^{th} absorber's thickness

The X-ray image is a summation image ("X-ray image", "radiographic image", "roentgenogram"). Contrast arises due to spatially varying attenuation.




Improving X-ray imaging I.

Increasing contrast: contrast agents

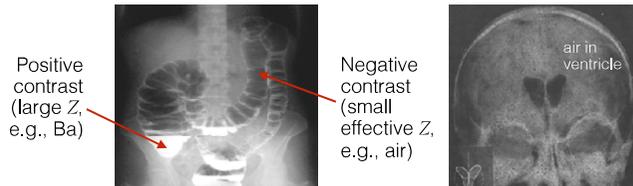

Enhancing sensitivity: intensifier

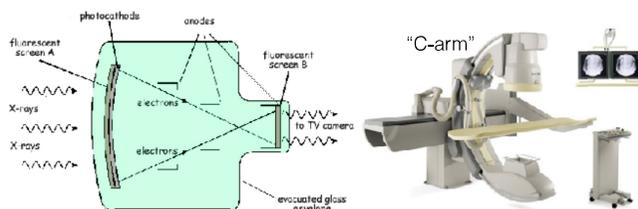


Background subtraction: "Digital Subtraction Angiography" (DSA)



Improving X-ray imaging II. Spatial resolution

Bi-directional X-ray imaging

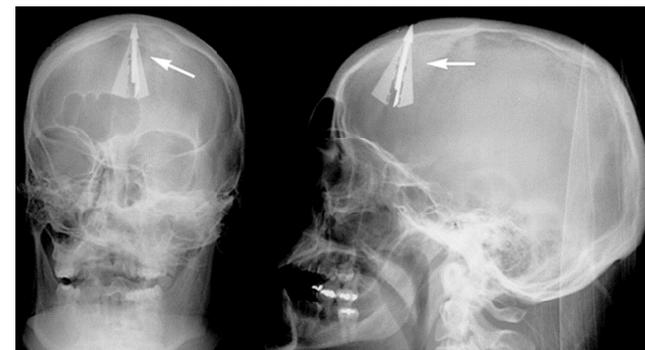


Bi-directional cranial X-ray of an individual who tried to commit suicide with a crossbow.

Improving X-ray imaging: the CAT scanner


History

- Röntgen, Hounsfield and Cormack
- 1967: first CAT scan
- 1972: prototype
- 1974: first clinical CAT image (head)
- 1976: whole body CAT scan
- 1979: Nobel-prize
- 1990: spiral CAT scanner
- 1992: multislice CAT scanner
- 2006: 64 slice (and more...)
- multiple and hybrid modes: SPECT-CT, PET-CT, Dual-source CT

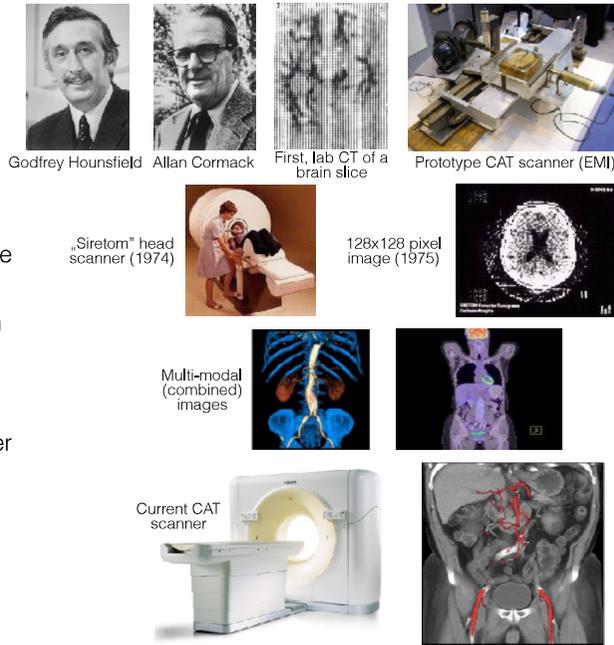

CT Foundations I: determination of μ

Objective: to determine the attenuation coefficient (μ_x) of the individual volume elements (voxels)

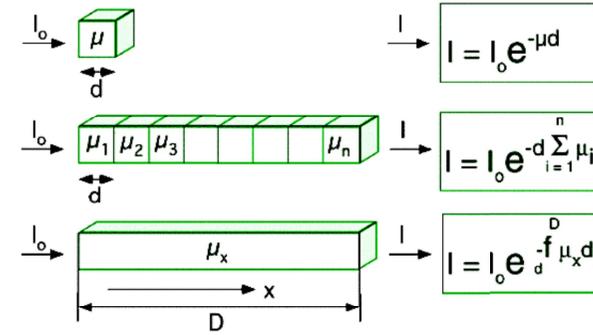


μ_x : linear attenuation coefficient
 d_x : size of the voxel

CT Image: Density matrix


$$N_{CT} = 1000 \frac{\mu - \mu_w}{\mu_w}$$

μ : attenuation coefficient of voxel
 μ_w : attenuation coefficient of water

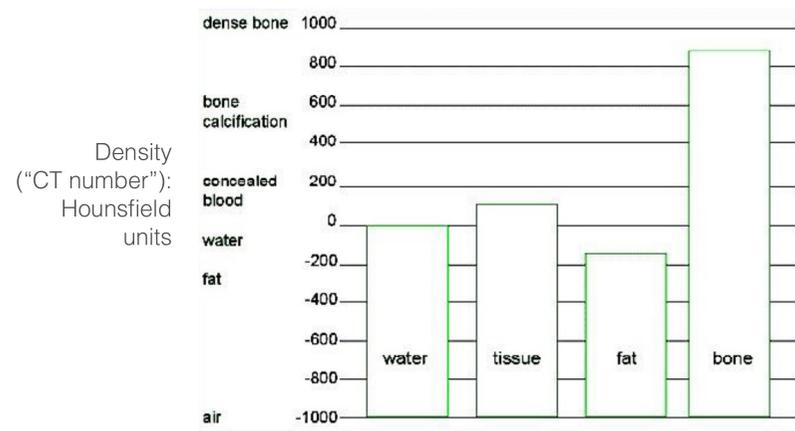


CT Foundations II: scanning

Scanning in transaxial tomographic slices

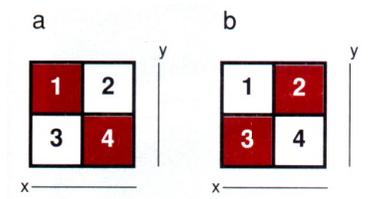


It is not possible to distinguish **a** from **b** in a bi-directional image

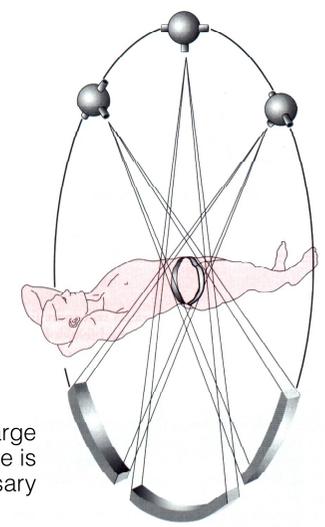

Scanning along as large angular resolution as possible is necessary



Scanning techniques evolved through generations

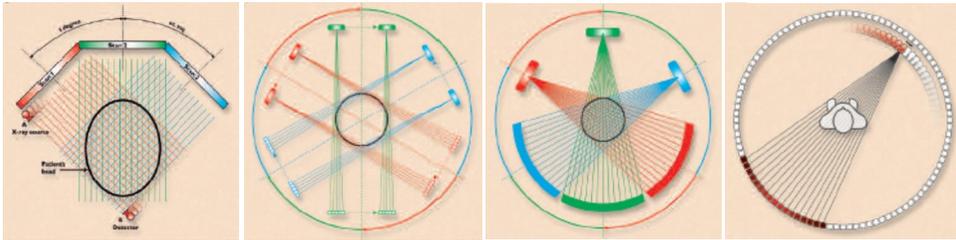


- I. Generation.** There is a single moving source and a single moving detector, each translating linearly, then rotated.
- II. Generation.** There are a small number of beams (approximately 8 to 30) in a narrow fan configuration with the same translate-rotate motion used in first generation machines. Each linear traverse produces several projections at differing angles, one view for each X-ray beam.
- III. Generation.** There are a large number of X-ray beams (approximately 500 to 700) in a wide fan configuration. Both the X-ray tube and the detectors rotate.
- IV. Generation.** There are an intermediate number of X-ray beams (approximately 50 to 200) in a wide fan configuration with a rotating X-ray tube and a stationary circular array of approximately 600 to 2,400 detectors surrounding the patient.

Current CT's use spiral (helical) scanning

Source-detector pair rotates constantly

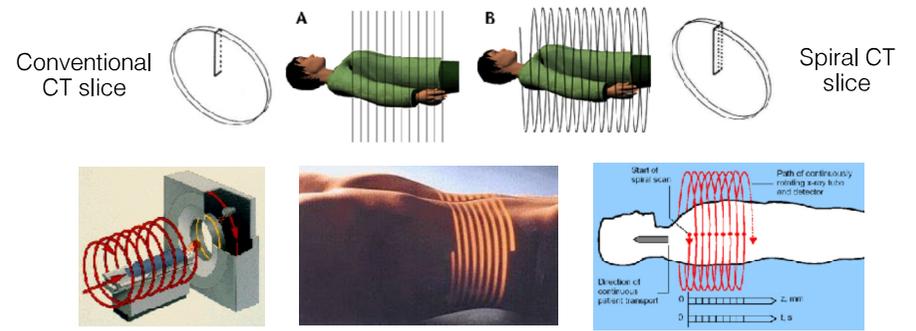


Multi-detector CT (MDCT)

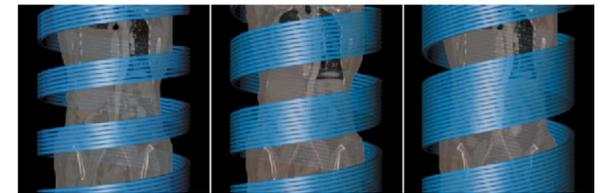



Multi-slice CT (MSCT)

CT foundations III: Image Reconstruction


1. Algebraic reconstruction techniques
2. Direct Fourier reconstruction
3. „Filtered Back Projection“ (current method)

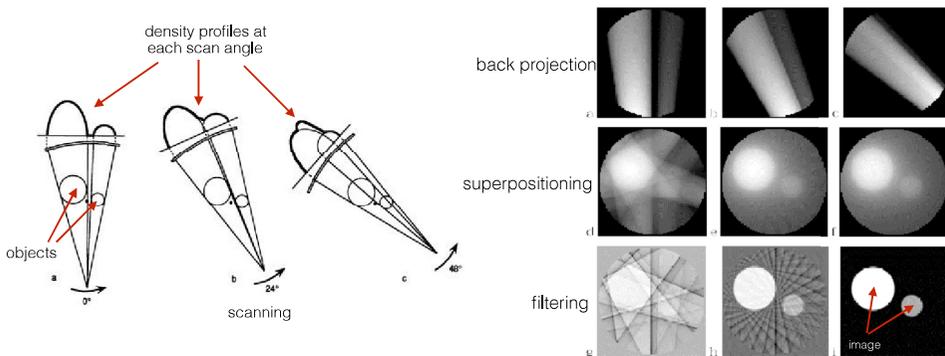

Contrast manipulation of CT Image „Windowing“

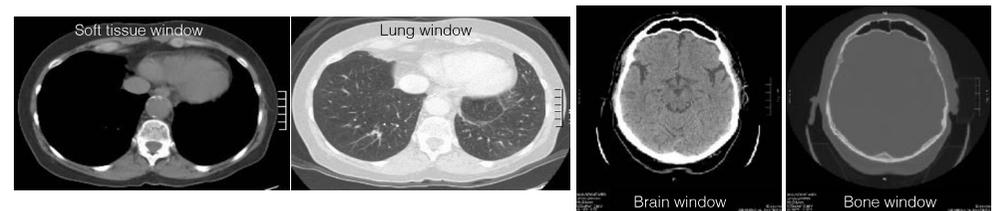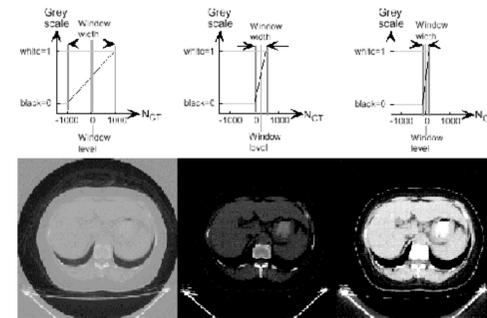

Modern CAT scanning

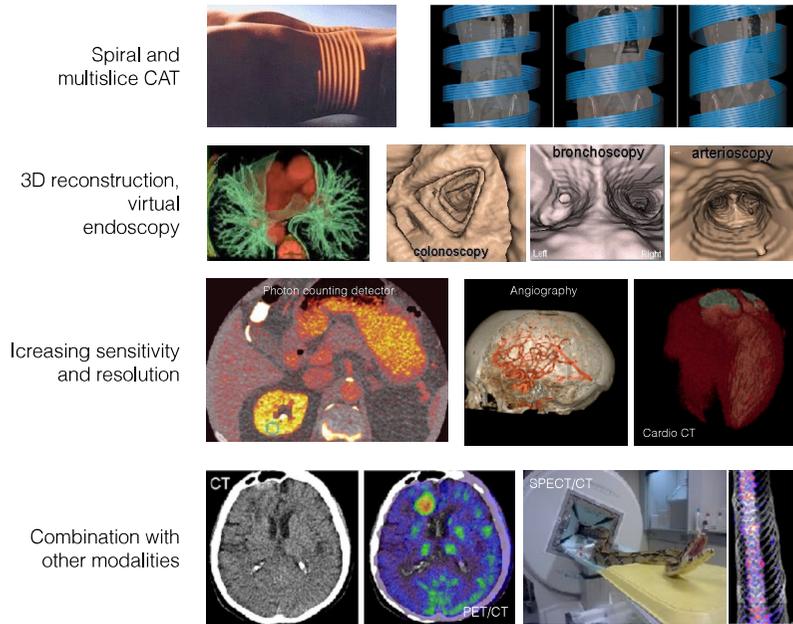


Summary of CT scanning (CAT)



- Tomographic digital imaging method that uses X-rays
- Principle: displaying differences in X-ray absorbance by the different points of the tomographic slice
- Conventional (outdated) technique: one slice – 2 - 4 sec, entire examination: 5 - 15 perc
- Spiral CT technique: one slice – 1 - 1.5 sec, entire examination: 30 - 60 sec (+ preparation)
- Multidetector spiral CT (4-64 detector array): one slice – 0.4 - 1 sec, entire examination: 5 - 15 sec

Absorptiometry

Dual-energy X-ray absorptiometry (DXA or DEXA)




- Most important method for measuring bone density
- Characteristic X-ray is used as source
- Two different photon energies are employed
- Low dose is applied
- Whole-body scan is recorded
- Densities of distinct areas (e.g., femur, spine) are compared with reference databases
- Bone Mineral Density (BMD) calculated
- T-score is established

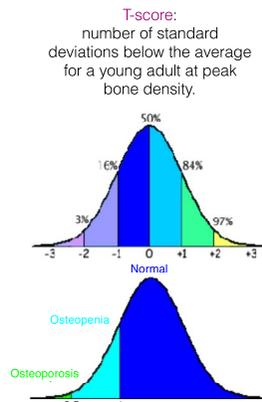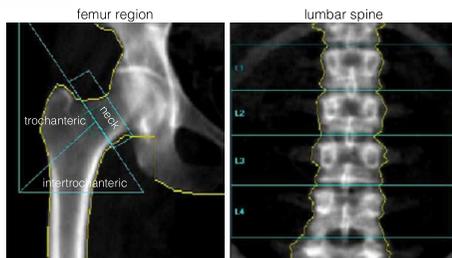


Generating high-energy X-ray

Linear accelerator (Linac)

- Charged particle (electron, proton) accelerated between electrodes (but not inside the electrode).
- Velocity of particle increases in steps.
- Electrode polarity is alternating.
- Electrodes are gradually longer (l_i increases) in order to maintain synchrony.
- Accelerated particles are directed at suitable target material (to generate X-ray).

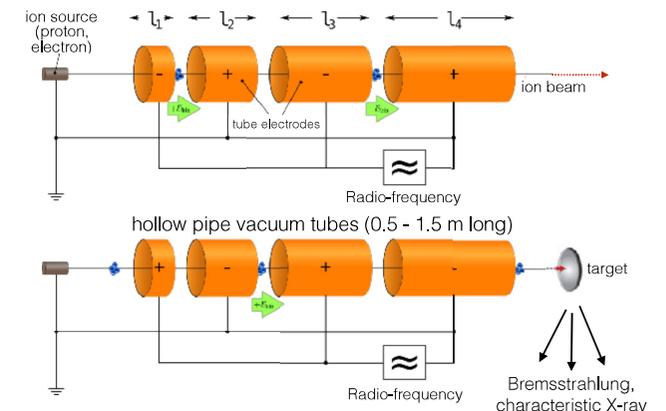

Linac-based radiation therapy

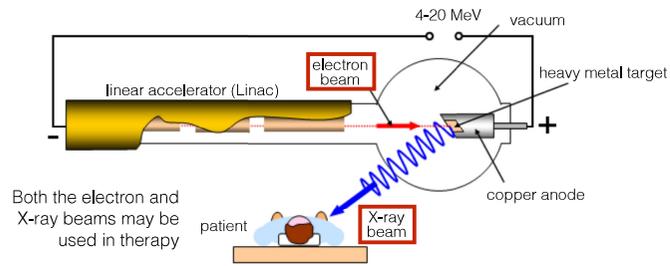

Both the electron and X-ray beams may be used in therapy



Modern hospital Linac

Advantages:


- Radiation may be turned on and off
- No contaminating radioactivity



First patient (Gordon Isaacs) treated with Linac radiation therapy (electron beam) for retinoblastoma (1955)

Ring-shape particle accelerators

Cyclotron

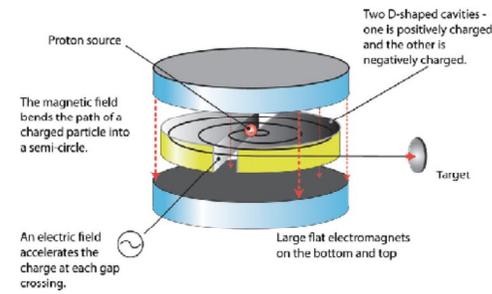


- Lorentz forces keep particles on circular path (causes limitations)
- Few tens of MeV particles are generated
- Used for generating positron-emitting isotopes (PET)
- Clinical cyclotrons in PET centers



11 MeV medical cyclotron

Synchrotron

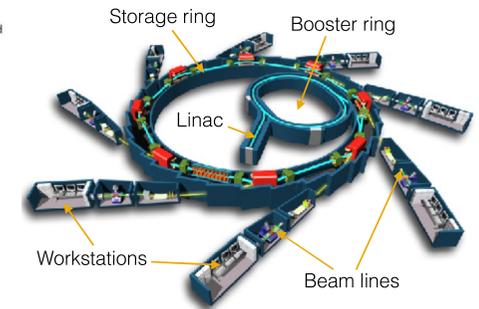

- Very high energy particles can be generated (GeV)
- Relativistic speeds can be achieved (near light speed)
- X-rays used for high-resolution structural research
- Few facilities around the world (Grenoble, Chicago, etc.)



J.D. Watson and C.F. Crick, and the first x-ray image of DNA (1953)