

X-ray

Applications

X-ray



Wilhelm Konrad Röntgen
(1845-1923)
Nobel prize in physics, 1901




Hand mit Ringen (Hand with Ring): print
of Wilhelm Röntgen's first "medical" X-
ray, of Anna Bertha Ludwig

X-ray applications


- Diagnostic imaging
The X-ray image
Improvements of X-ray imaging
CAT scanning
- Absorptiometry
Bone density testing
- Therapy
Generation of high-energy X-ray
Tumor irradiation

X-ray absorption

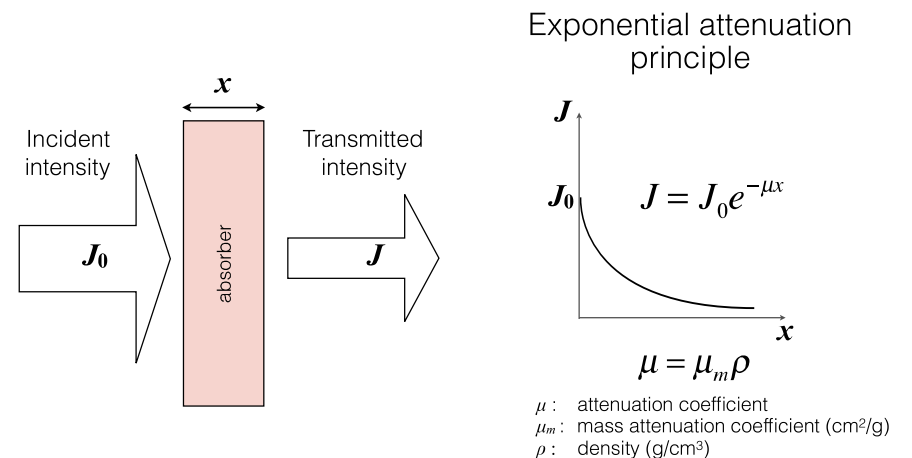

μ_m is the sum of the mass attenuation coefficients
of the different absorption mechanisms.

Attenuation mechanisms


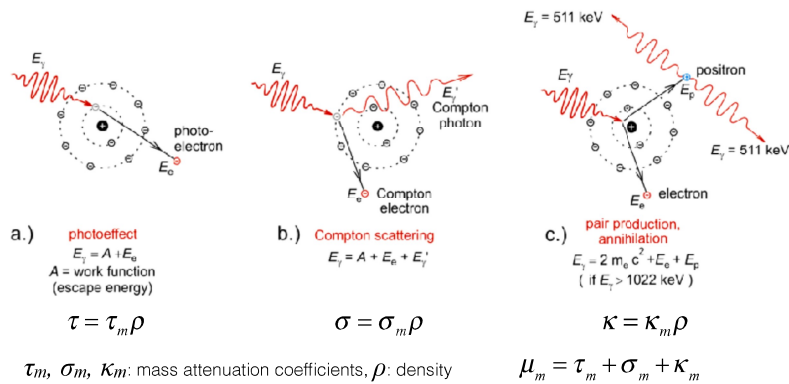


Mechanism	Photon energy (ϵ) dependence of the mass attenuation coefficient	Atomic number (Z) dependence of the mass attenuation coefficient	Relevant energy range in soft tissue
Photoeffect	$\sim 1 / \epsilon^3$	$\sim Z^3$	10 - 100 keV
Compton scatter	falls gradually with ϵ	$\sim Z/A$ (A : mass number)	0.5 - 5 MeV
Pair production	rises slowly with ϵ	$\sim Z^2$	$> 5 \text{ MeV}$

Diagnostic X-ray:

1. Contrast mechanism between soft tissue and bone: photoeffect ($\sim Z^3$)
2. Contrast mechanism within soft tissue: Compton-scatter ($\sim \rho$)

Principles of X-ray imaging

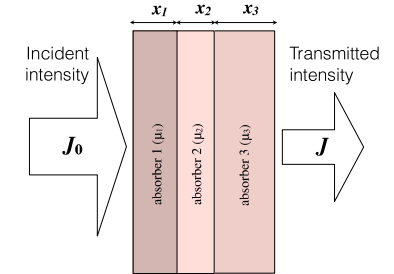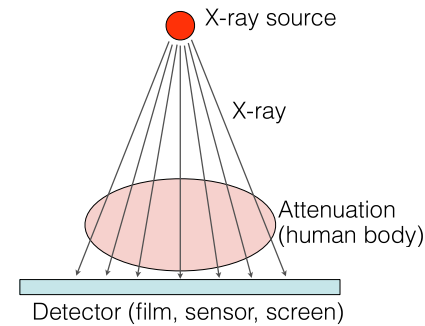


$$J = J_0 e^{-(\mu_1 x_1 + \mu_2 x_2 + \mu_3 x_3 + \dots)}$$

$$\lg \frac{J_0}{J} = (\mu_1 x_1 + \mu_2 x_2 + \mu_3 x_3 + \dots) \cdot \lg e$$


μ_n : n^{th} absorber's attenuation coefficient
 x_n : n^{th} absorber's thickness

The X-ray image is a summation image ("X-ray image", "radiographic image", "roentgenogram"). Contrast arises due to spatially varying attenuation.




Improving X-ray imaging I.

Increasing contrast: contrast agents

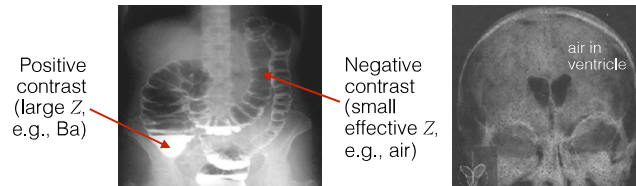

Enhancing sensitivity: intensifier

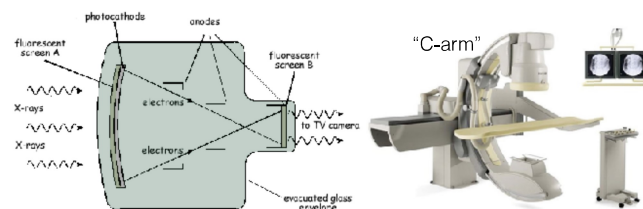


Background subtraction: "Digital Subtraction Angiography" (DSA)



Improving X-ray imaging II. Spatial resolution

Bi-directional X-ray imaging

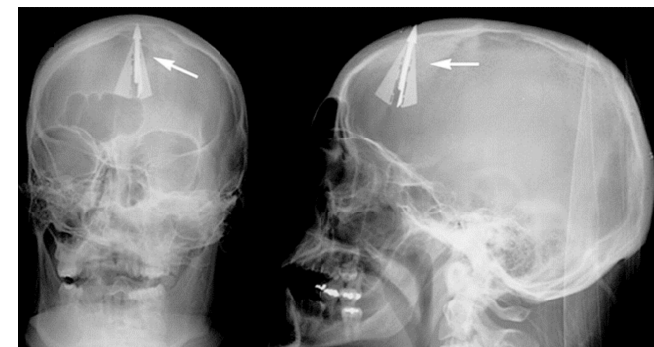


Bi-directional cranial X-ray of an individual who tried to commit suicide with a crossbow.

Improving X-ray imaging: the CAT scanner

History


- Röntgen, Hounsfield and Cormack
- 1967: first CAT scan
- 1972: prototype
- 1974: first clinical CAT image (head)
- 1976: whole body CAT scan
- 1979: Nobel-prize
- 1990: spiral CAT scanner
- 1992: multislice CAT scanner
- 2006: 64 slice (and more...)
- multiple and hybrid modes: SPECT-CT, PET-CT, Dual-source CT

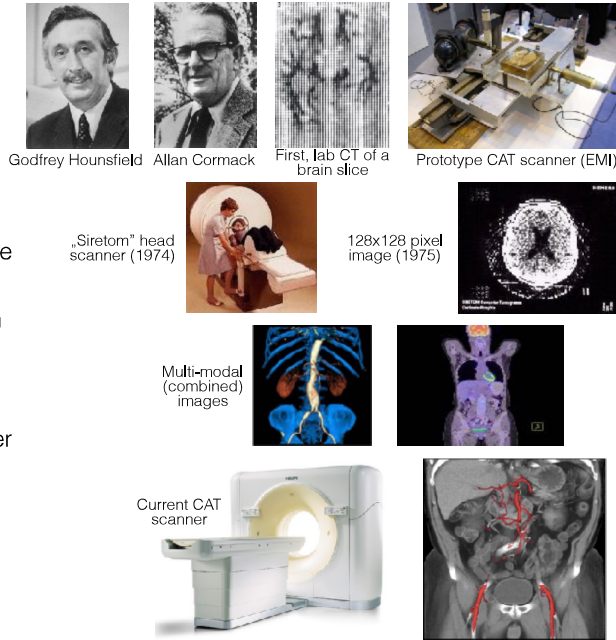

CT Image: Density matrix


$$N_{CT} = 1000 \frac{\mu - \mu_w}{\mu_w}$$

μ : attenuation coefficient of voxel
 μ_w : attenuation coefficient of water

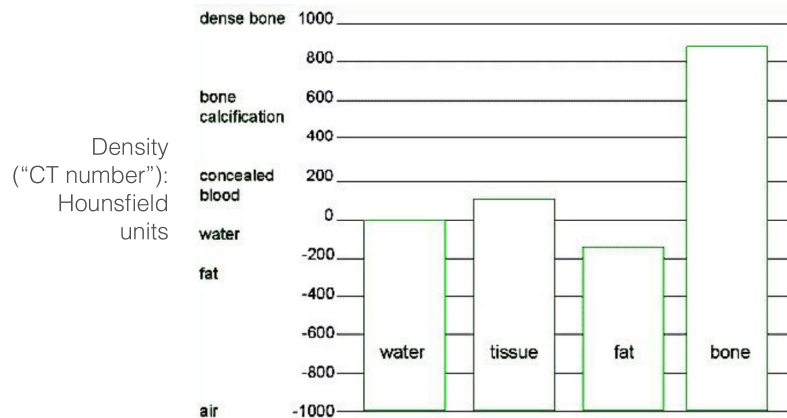

CT Foundations I: determination of μ


Objective: to determine the attenuation coefficient (μ_x) of the individual volume elements (voxels)

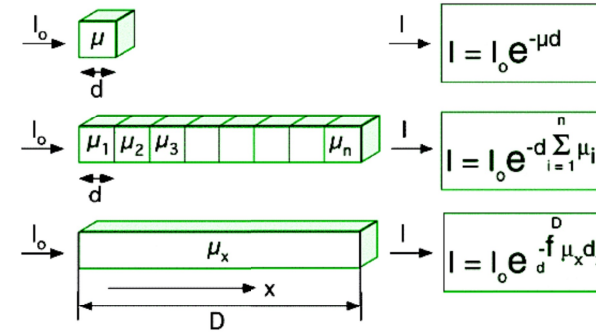


μ_x : linear attenuation coefficient
 d_x : size of the voxel

CT Foundations II: scanning

Scanning in transaxial tomographic slices

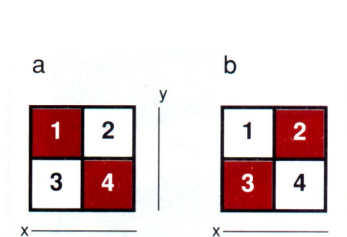


It is not possible to distinguish **a** from **b** in a bi-directional image

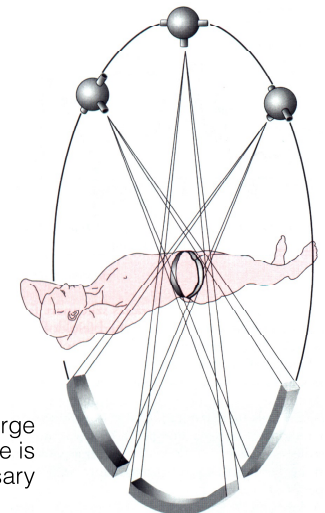

Scanning along as large angular resolution as possible is necessary



Scanning techniques evolved through generations

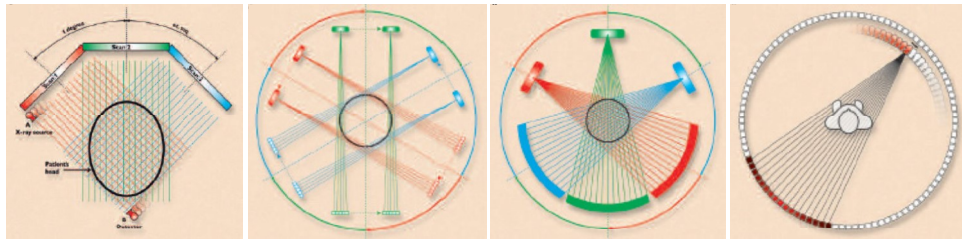


- I. Generation.**
There is a single moving source and a single moving detector, each translating linearly, then rotated.
- II. Generation.**
There are a small number of beams (approximately 8 to 30) in a narrow fan configuration with the same translate-rotate motion used in first generation machines. Each linear traverse produces several projections at differing angles, one view for each X-ray beam.
- III. Generation.**
There are a large number of X-ray beams (approximately 500 to 700) in a wide fan configuration. Both the X-ray tube and the detectors rotate.
- IV. Generation.**
There are an intermediate number of X-ray beams (approximately 50 to 200) in a wide fan configuration with a rotating X-ray tube and a stationary circular array of approximately 600 to 2,400 detectors surrounding the patient.

Current CT's use spiral (helical) scanning

Source-detector pair rotates constantly

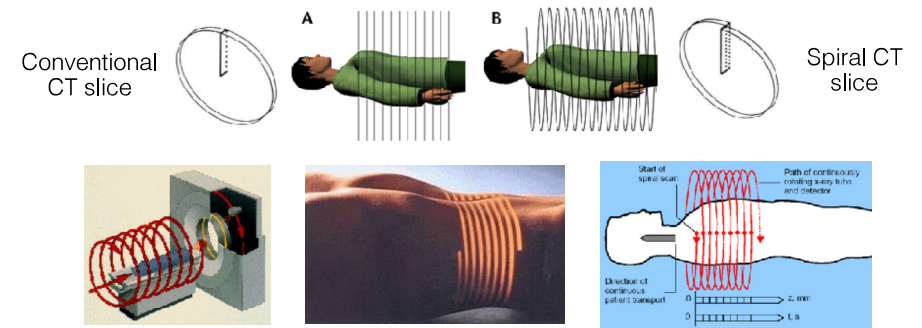


Multi-detector CT (MDCT)

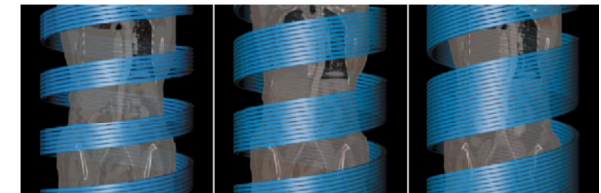



Multi-slice CT (MSCT)

CT foundations III: Image Reconstruction


1. Algebraic reconstruction techniques
2. Direct Fourier reconstruction
3. „Filtered Back Projection“ (current method)

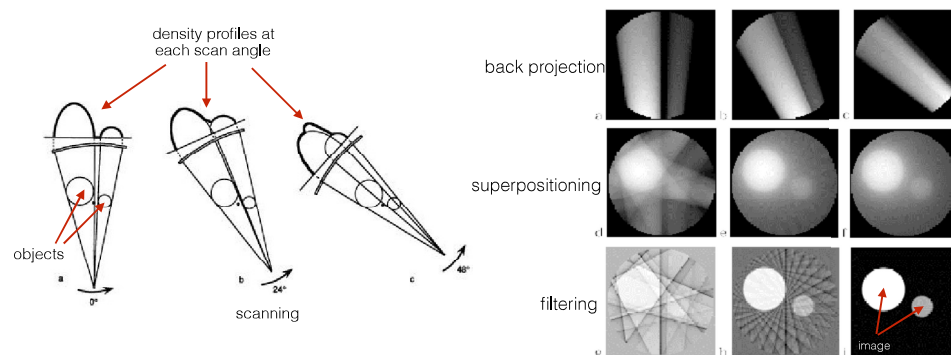

Contrast manipulation of CT Image „Windowing“

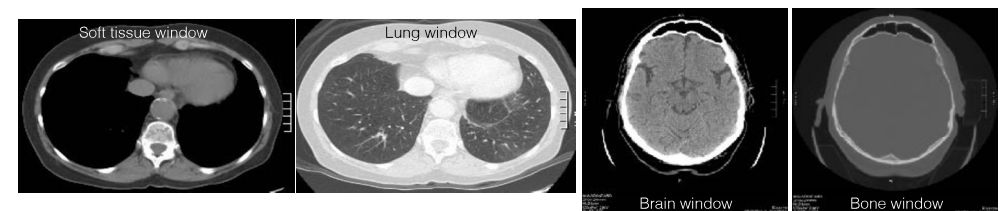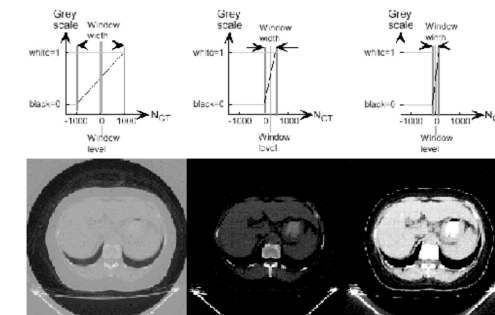

Modern CAT scanning

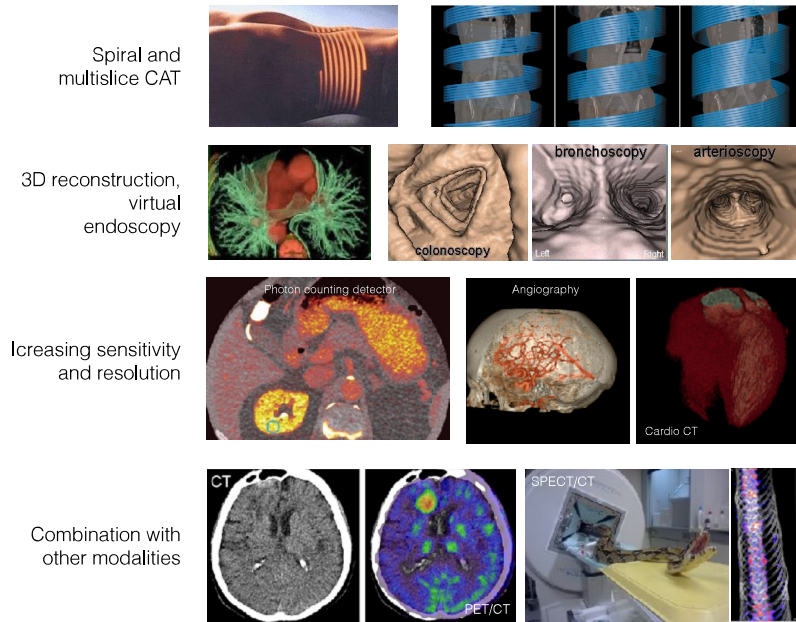


Summary of CT scanning (CAT)



- Tomographic digital imaging method that uses X-rays
- Principle: displaying differences in X-ray absorbance by the different points of the tomographic slice
- Conventional (outdated) technique:
one slice – 2 - 4 sec,
entire examination: 5 - 15 perc
- Spiral CT technique:
one slice – 1 - 1.5 sec,
entire examination: 30 - 60 sec (+ preparation)
- Multidetector spiral CT (4-64 detector array):
one slice – 0.4 - 1 sec,
entire examination: 5 - 15 sec

Absorptiometry

Dual-energy X-ray absorptiometry (DXA or DEXA)




- Most important method for measuring bone density
- Characteristic X-ray is used as source
- Two different photon energies are employed
- Low dose is applied
- Whole-body scan is recorded
- Densities of distinct areas (e.g., femur, spine) are compared with reference databases
- Bone Mineral Density (BMD) calculated
- T-score is established

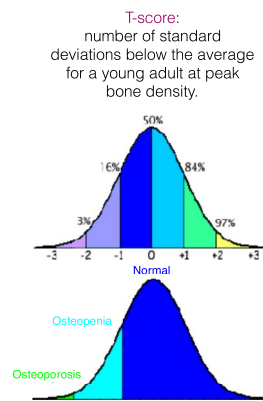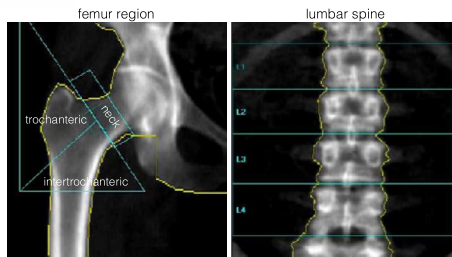


Generating high-energy X-ray

Linear accelerator (Linac)

- Charged particle (electron, proton) accelerated between electrodes (but not inside the electrode).
- Velocity of particle increases in steps.
- Electrode polarity is alternating.
- Electrodes are gradually longer (l_n increases) in order to maintain synchrony.
- Accelerated particles are directed at suitable target material (to generate X-ray).

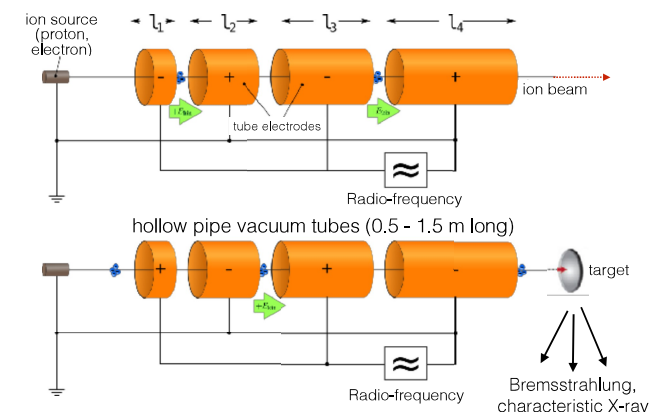

Linac-based radiation therapy

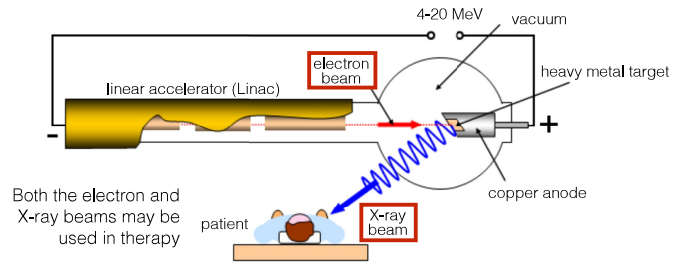

Modern hospital Linac




First patient (Gordon Isaacs) treated with Linac radiation therapy (electron beam) for retinoblastoma (1955)

Advantages:

- Radiation may be turned on and off
- No contaminating radioactivity

Ring-shape particle accelerators

Cyclotron

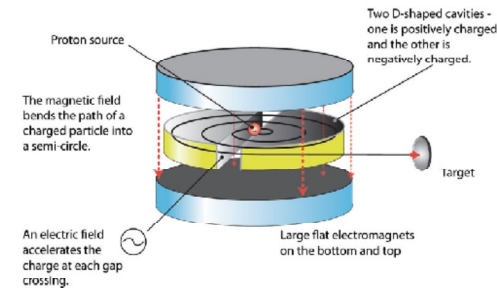


- Lorentz forces keep particles on circular path (causes limitations)
- Few tens of MeV particles are generated
- Used for generating positron-emitting isotopes (PET)
- Clinical cyclotrons in PET centers




11 MeV medical cyclotron

Synchrotron

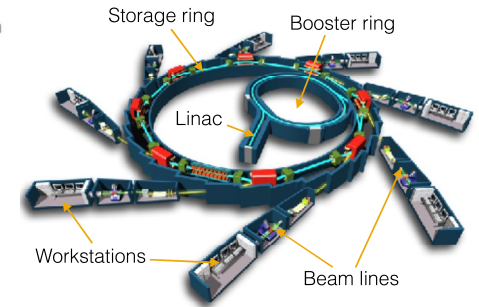

- Very high energy particles can be generated (GeV)
- Relativistic speeds can be achieved (near light speed)
- X-rays used for high-resolution structural research
- Few facilities around the world (Grenoble, Chicago, etc.)

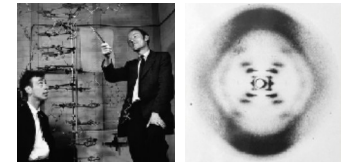

J.D. Watson and C.F. Crick, and the first x-ray image of DNA (1953)