

Special microscopic techniques

Dora Haluszka

2/11/2020




A brief history of microscopes




- Romans were looking through glass and testing it
- 1600s: Zacharias Jansen – first telescope/compound microscope



**Jansen
Microscope**

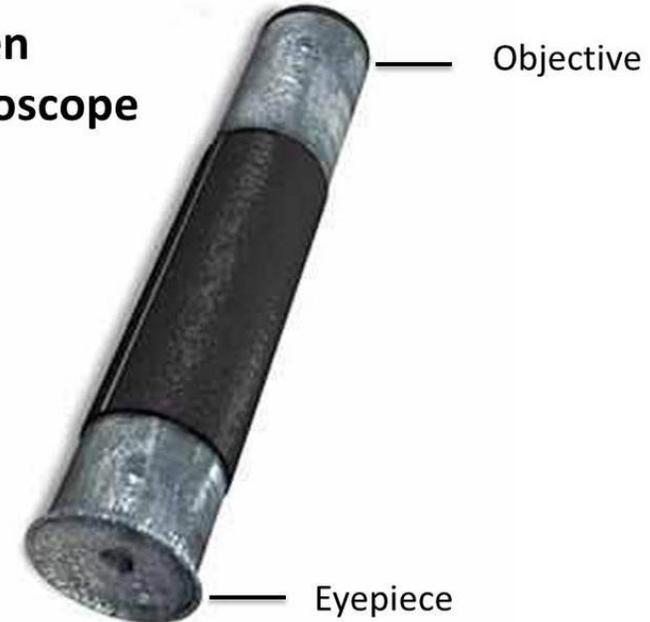



- 1667: Robert Hooke – „Micrographia”, cells of cork

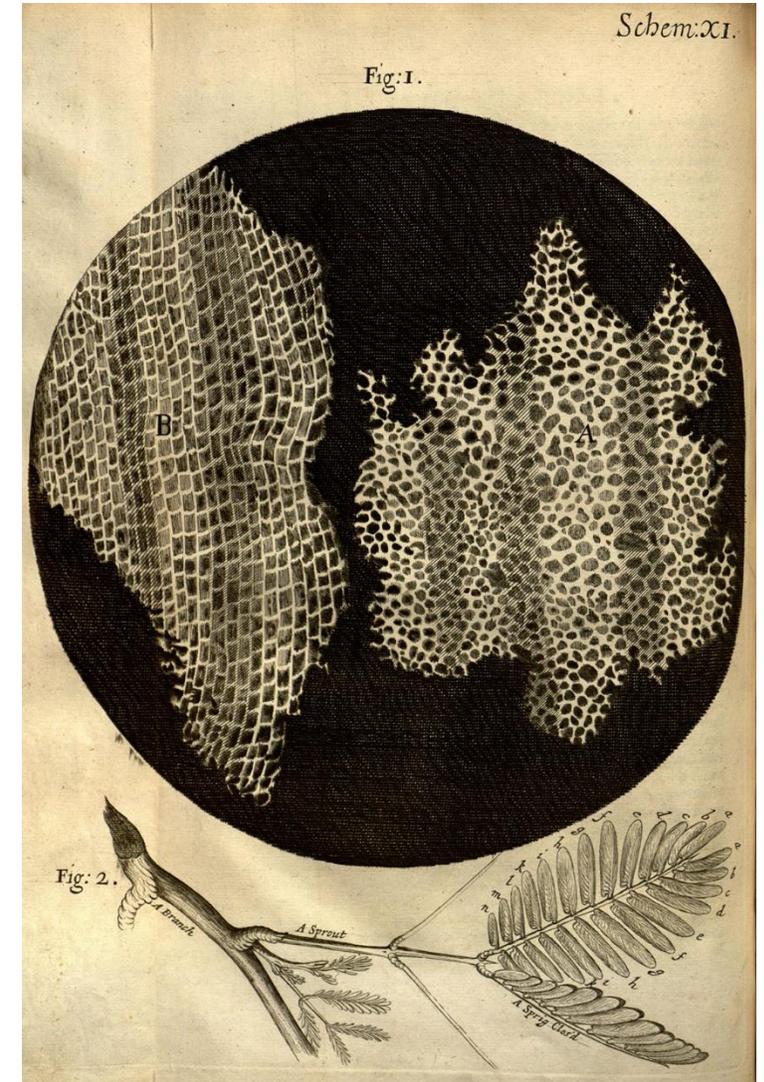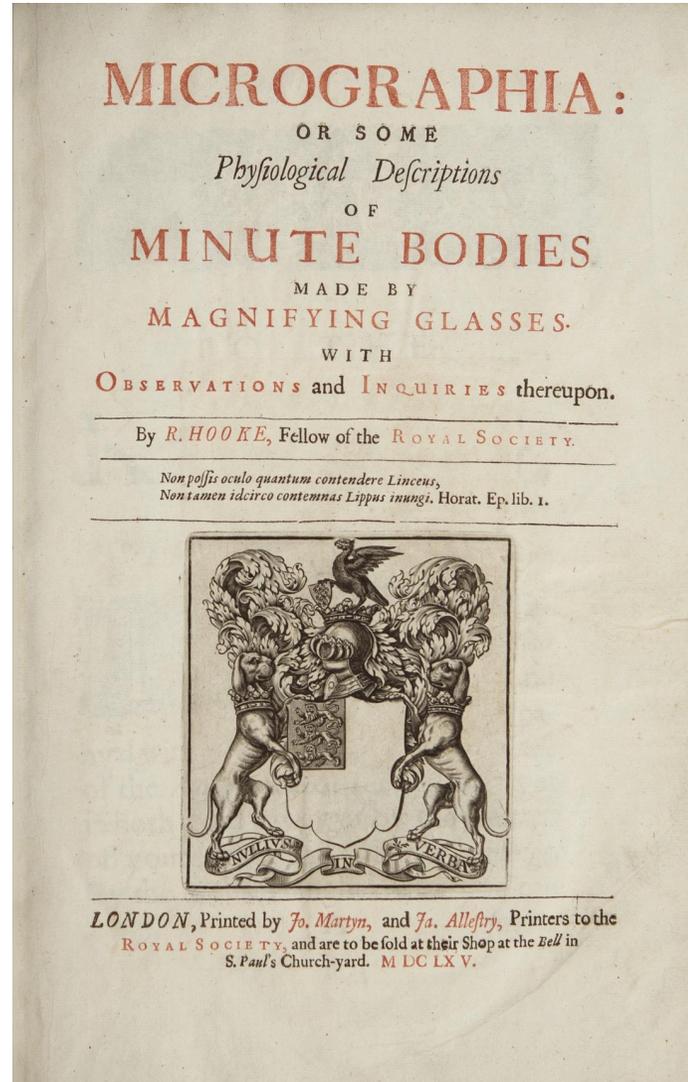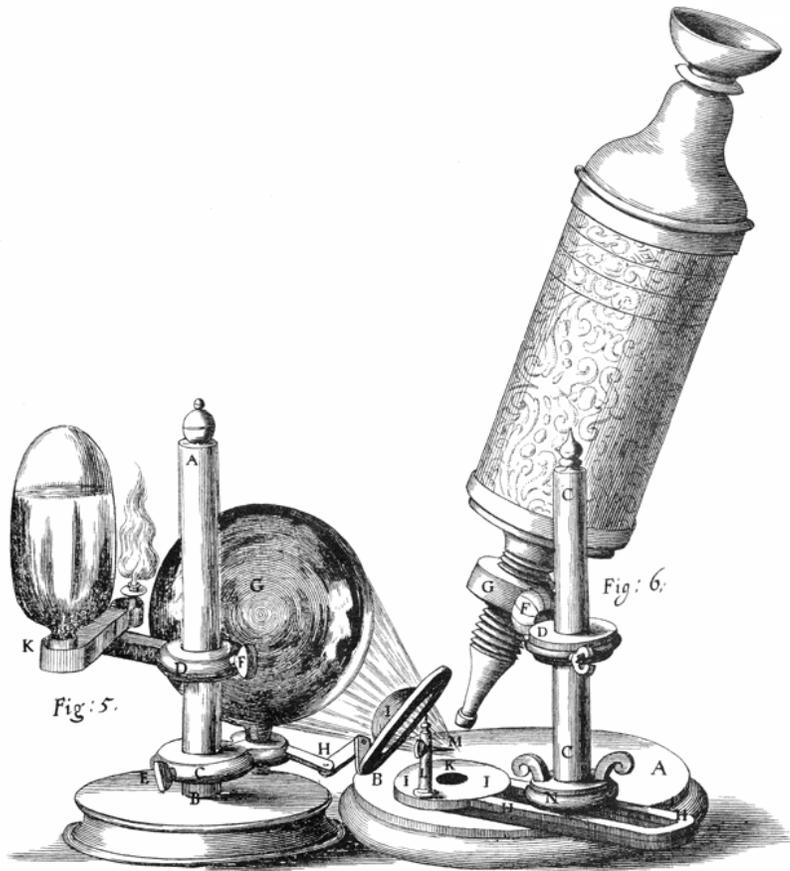



„The open universe”

- 1674: Antonie van Leeuwenhoek – make simple microscopes, 270 x magnification

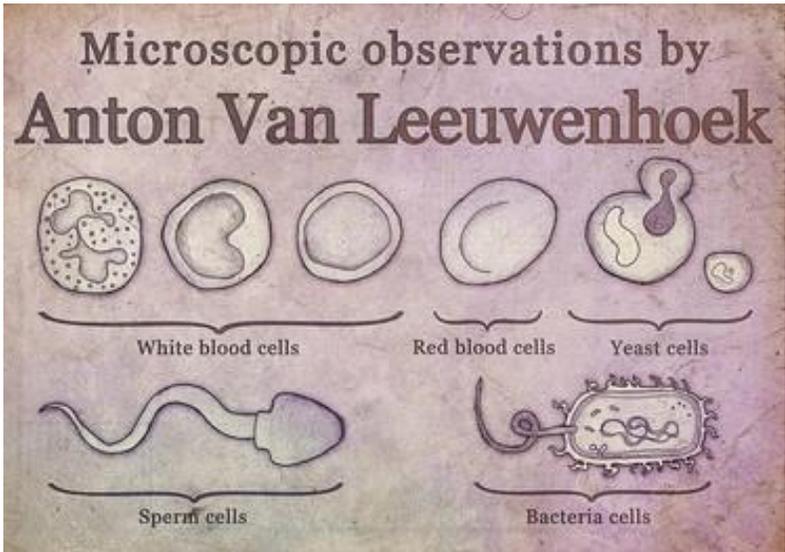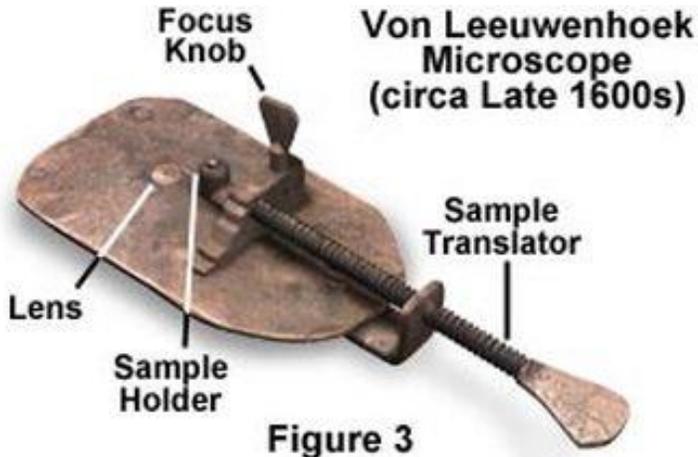


- Early 1800s
- Carl Zeiss – businessman in Jena – development of high quality microscope
- Ernst Abbe – He put the production of optical devices on scientific bases


Figure 2



Ernst Abbe (1840-1905)

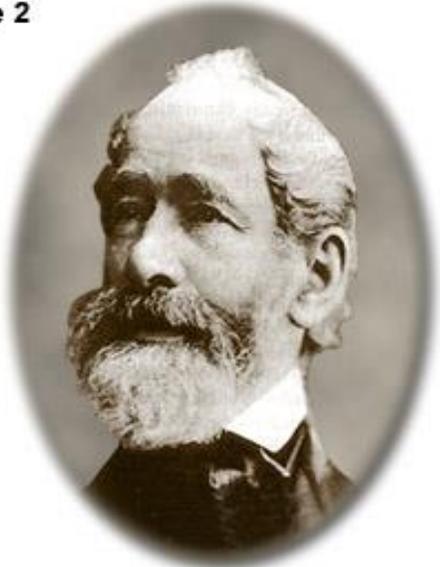


Carl Zeiss (1816-1888)

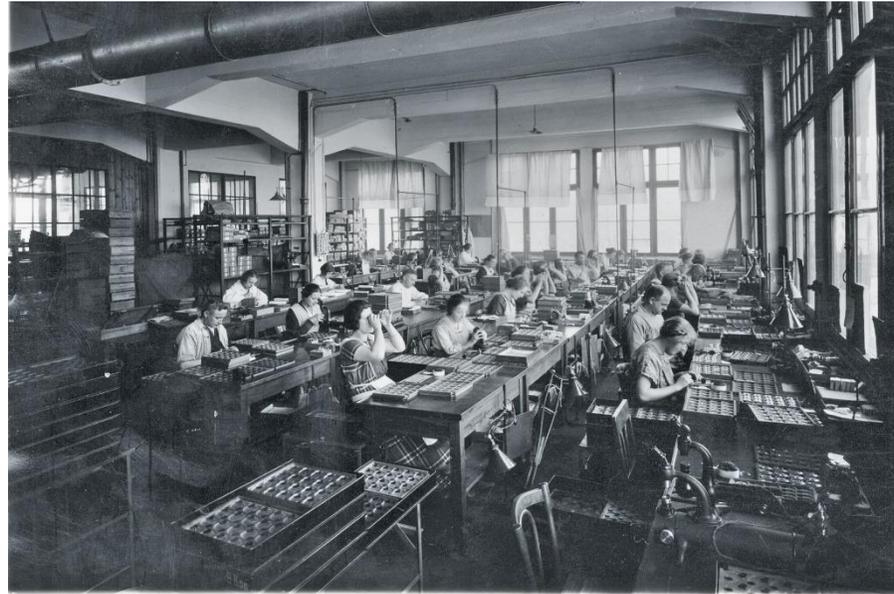


Microscope by Carl Zeiss (1879) with optics by Abbe

Fundamentals of wave optics

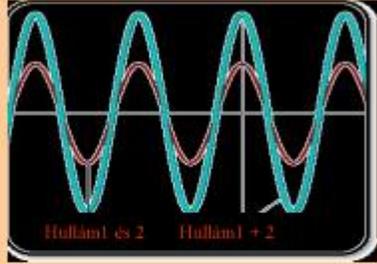

Similar phase

Constructive interference

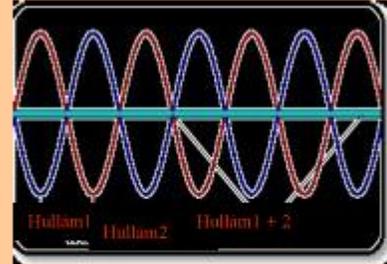


Opposite waves

Destructive interference



Young's experiment

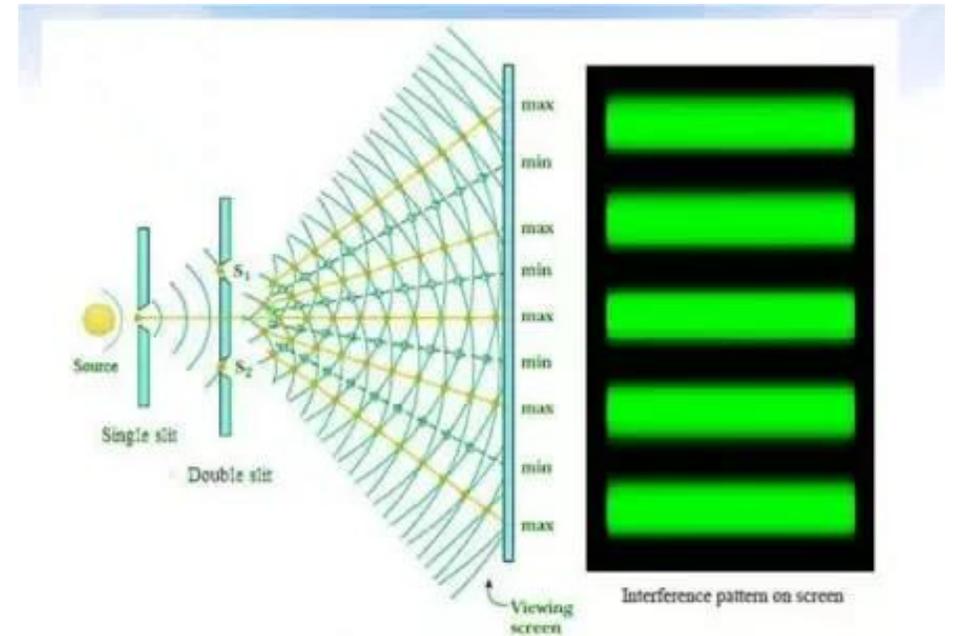

Resolution limit of microscope

1873: Ernst Abbe – resolution limit of light microscope


Abbe's principle: An optical system can resolve only those details of the specimen, which diffract light rays in a way that besides the principal maximum at least the first order diffraction rays are allowed to contribute to the image formation.



Ernst Abbe (1840-1905)

$$\delta = 0,61 \frac{\lambda}{n \sin \omega}$$

δ limit of resolution – distance between two object details which can be just resolved




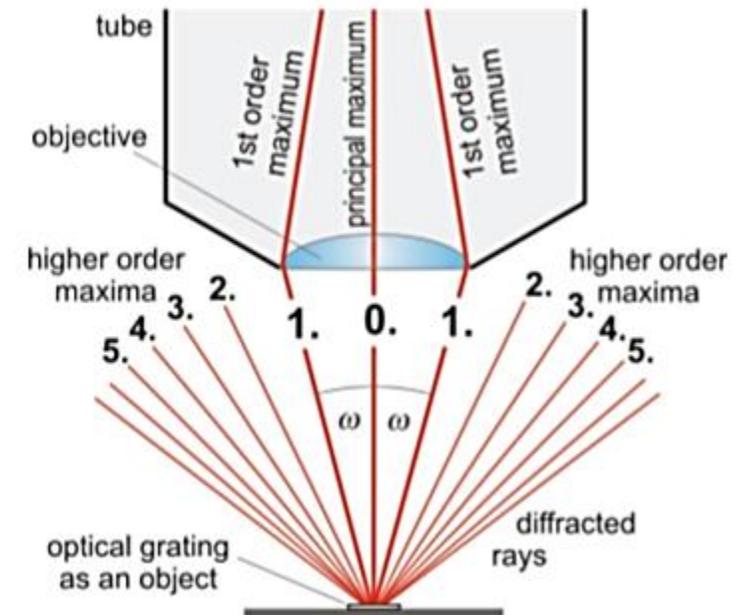


Airy disks – the evidence of wave character of light


The Airy disk is descriptions of the best-focused spot of light that a perfect lens with a circular aperture can make, limited by the diffraction of light.

Formation: the waves in same phase produce diffraction maximum (left) while the waves shifted by 180° produce diffraction minimum (right).

Point Spread Function (PSF): The objective focuses light in a volume and not into one point.

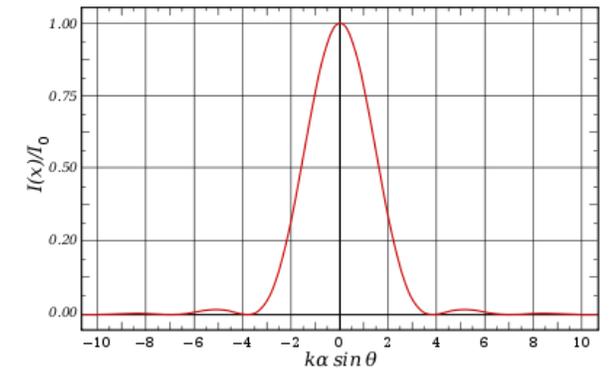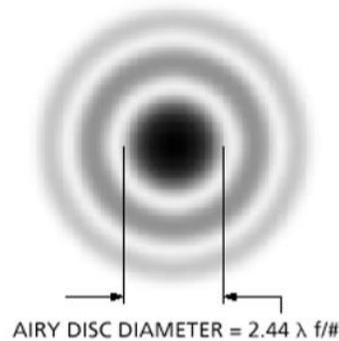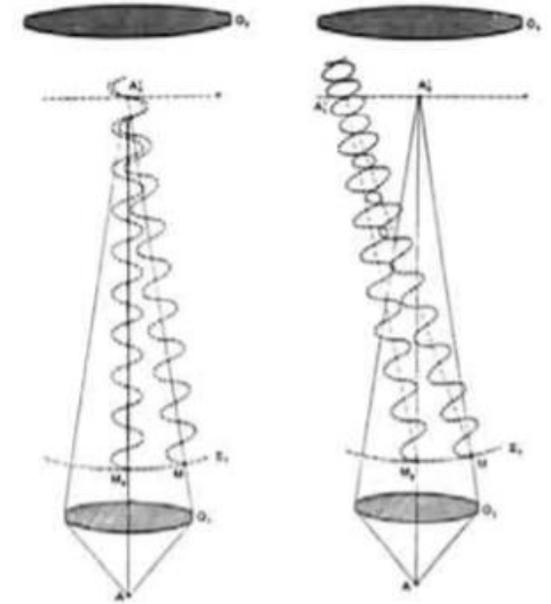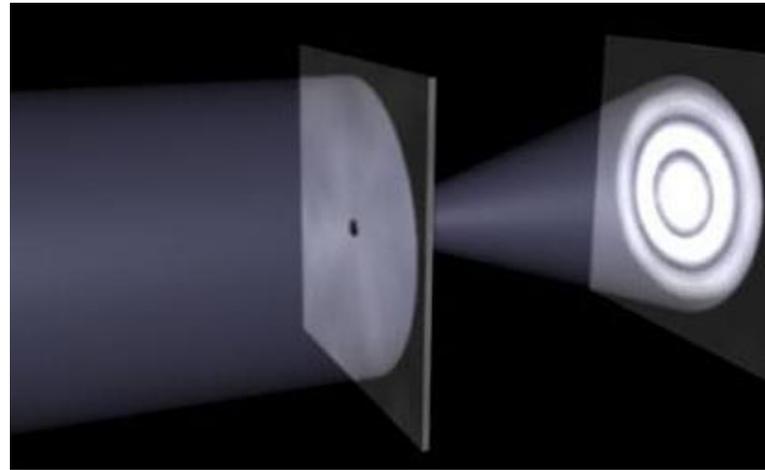

How can we distinguish two image points?

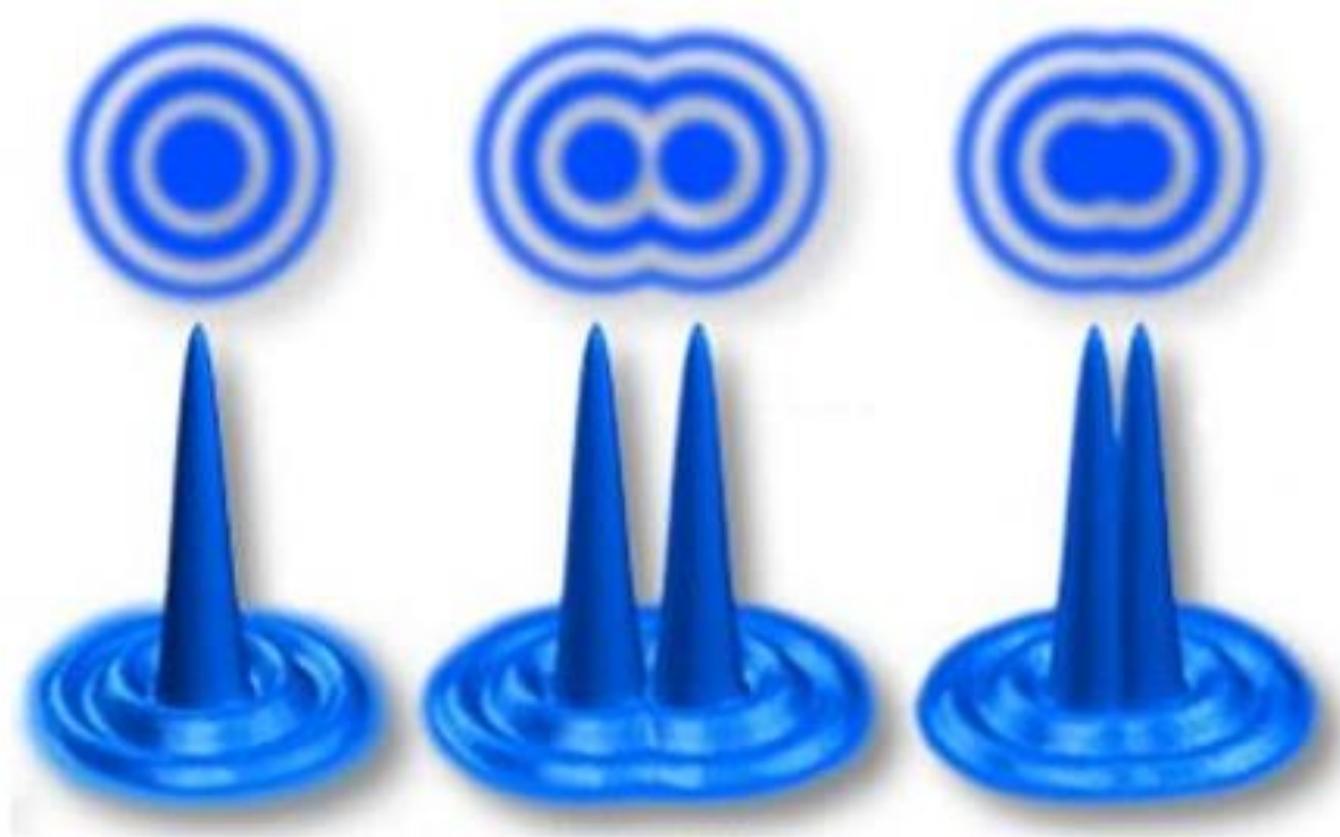


Rayleigh criterion:

Objects may be resolved if their corresponding Airy disk do not overlap.

Fluorescence microscope

Jablonski diagram

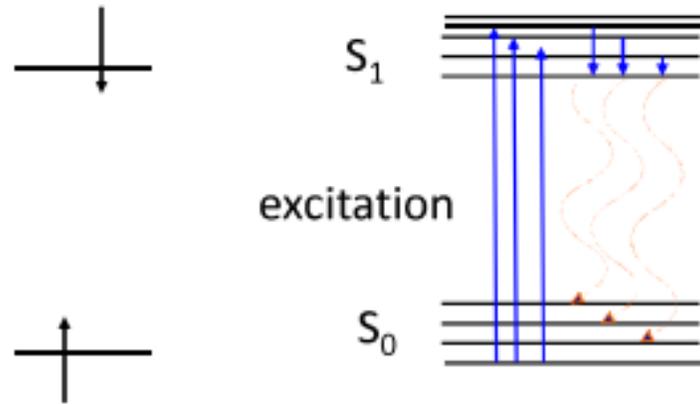

Non-radiant transitions

Light emission

Fluorescence

$$E_{\text{excitation}} \geq E_{\text{fluorescence}}$$

$$\lambda_{\text{excitation}} \leq \lambda_{\text{fluorescence}}$$

Stokes-shift



First excited singlet state

the spin states of
the electrons

sum of all e⁻ spin quantum
numbers=0

De-excitation by photon emission
between singlet states

Fluorescence microscope



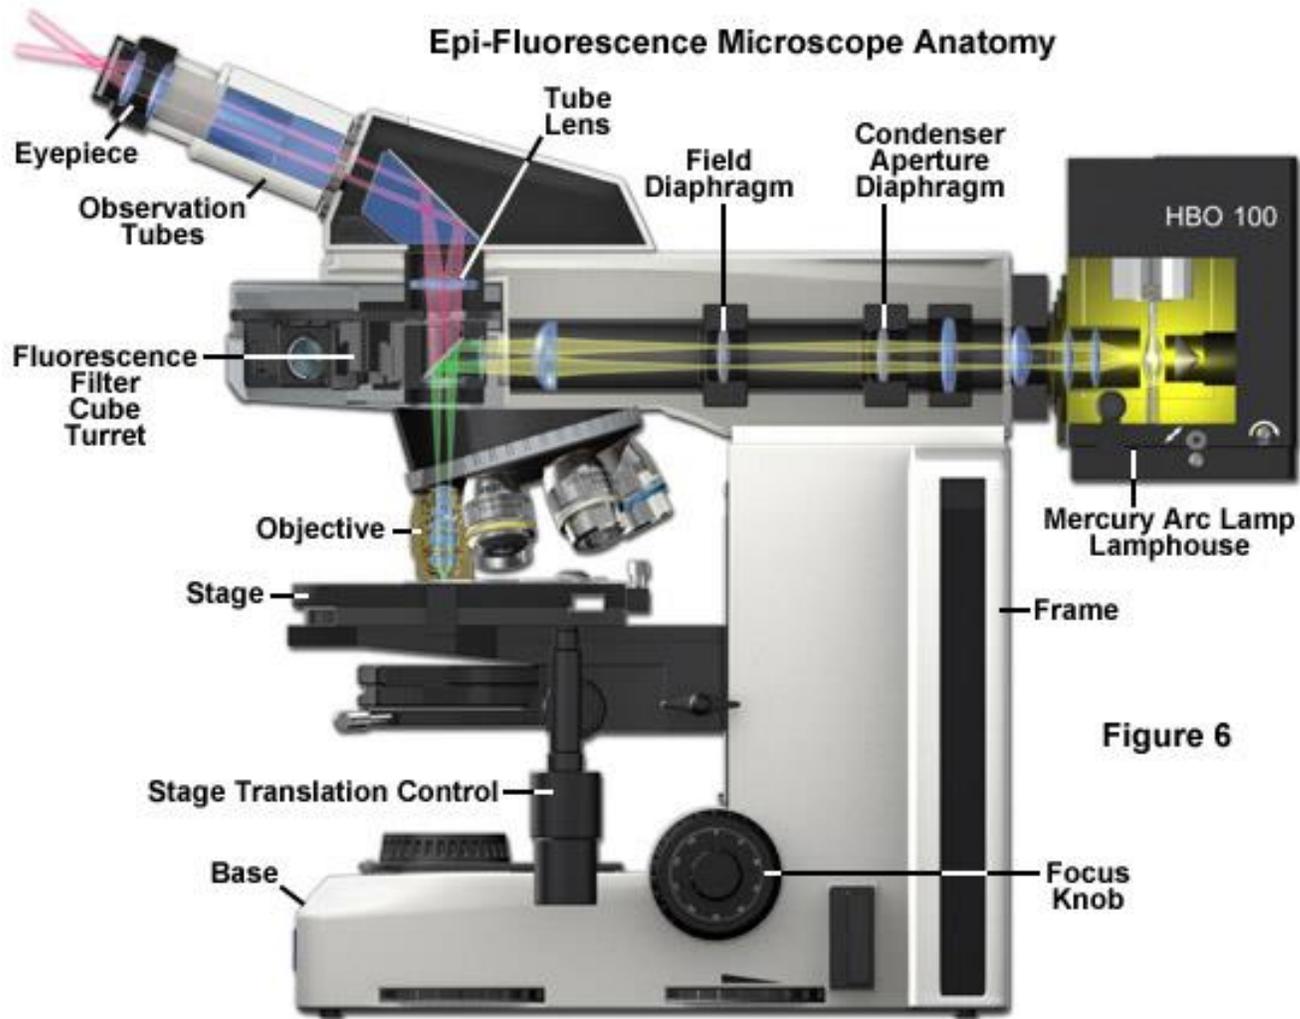


Figure 6

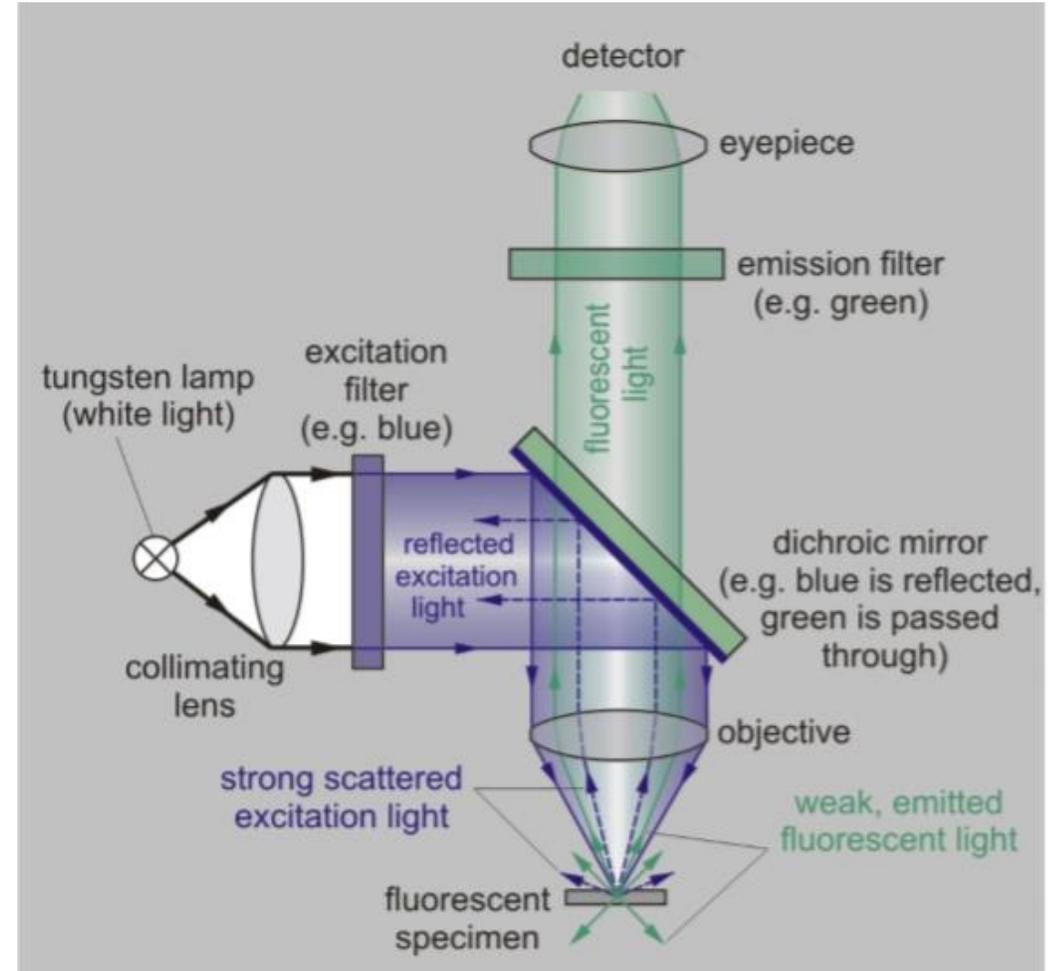

Light absorption and emission spectrum

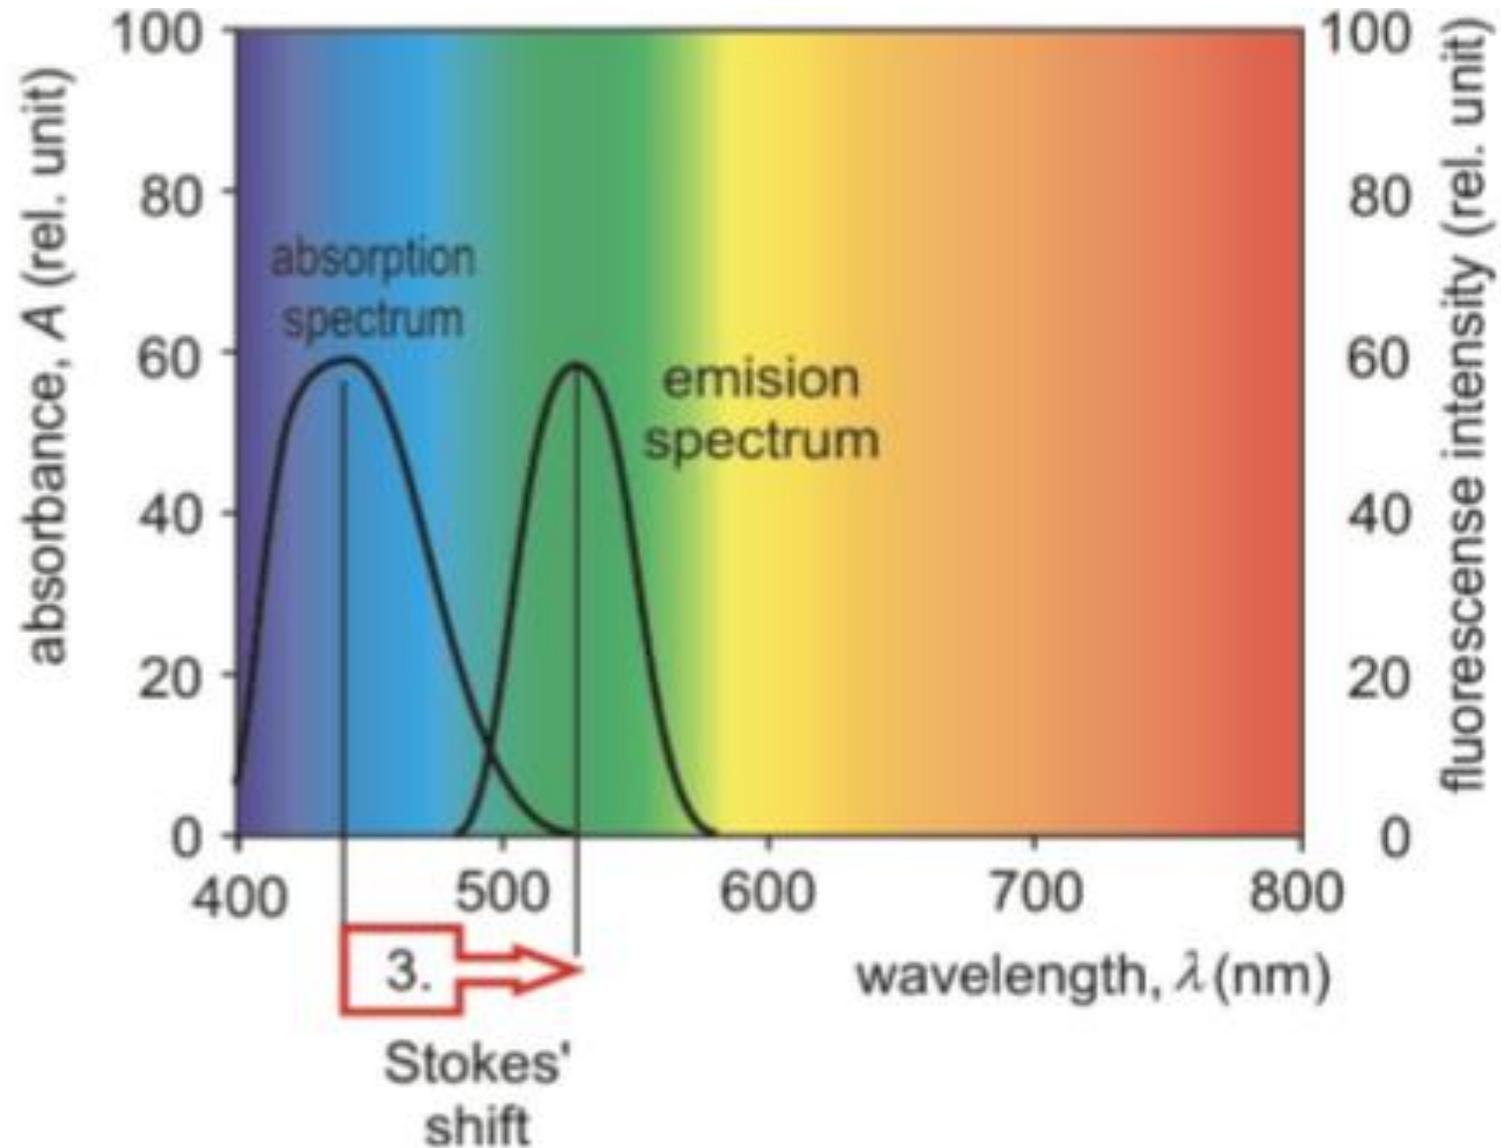

Source of fluorescence

- **Intrinsic** fluorophores:


tryptophan, tyrosine aminoacids, porphyrins

- **Extrinsic** fluorophores:


fluorescent dyes

The perfect fluorescent dye:


- Small
- Hydrophil
- Can be excited in the visible range
- Large Stokes-shift
- Specific
- No photoreactions

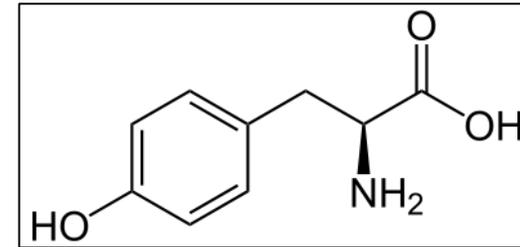


tyrosine

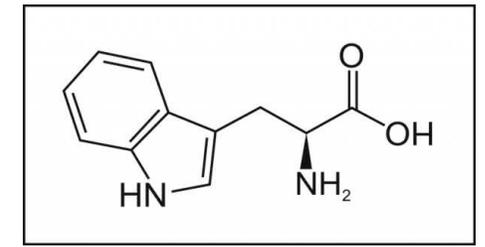


tryptophan

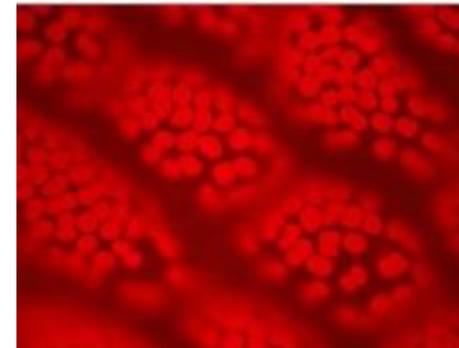

porphyrin fluorescence

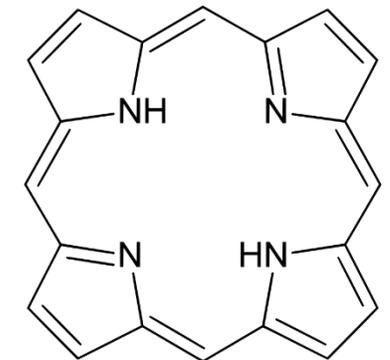


porphyrin

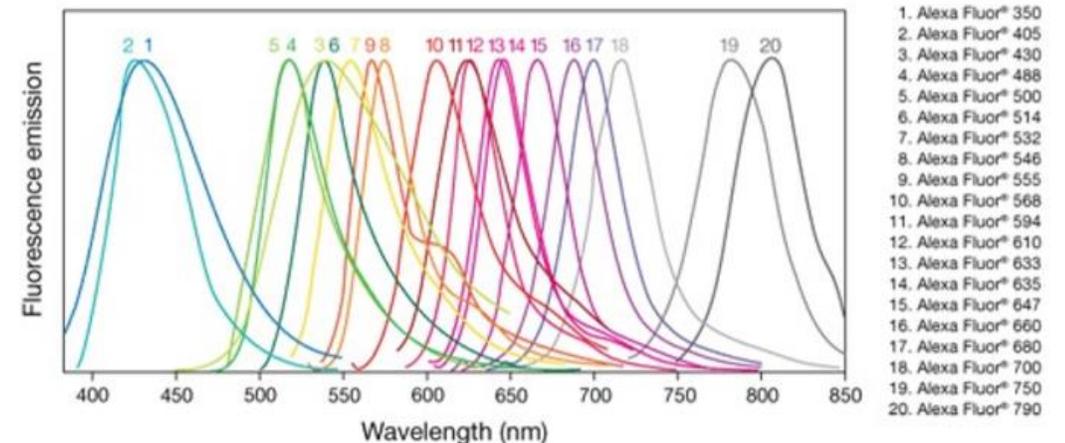



Fluorescent proteins

- Green Fluorescent Protein (GFP)
- first isolated from jellyfish (1960s)
- ~27 kDa, 238 aa, 11 strands β -barrel structure
- the central alpha helix contains the chromophore: Ser-65, Tyr-66, and Gly-67
- excitation: blue (475 nm) and UV (396 nm) light
- emission: 508 nm

- Used as tagging protein
- Small size – has no effect on the function of examined protein
- Transfected cells
- Transgene animals: all cell express the GFP

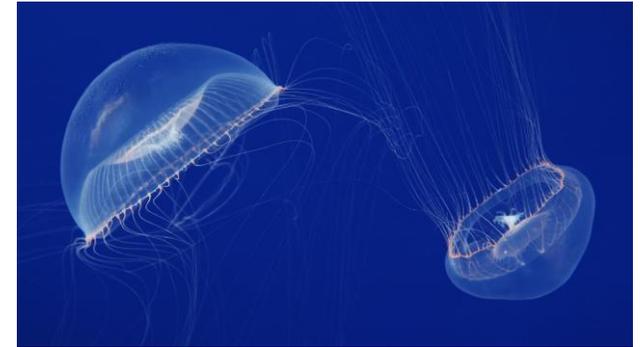


Aequorea victoria

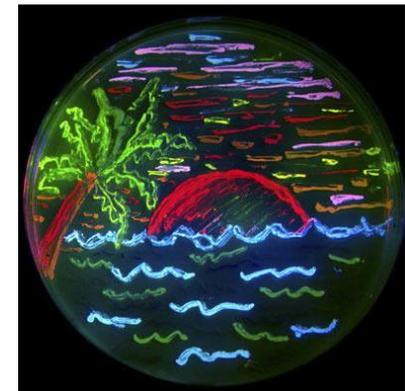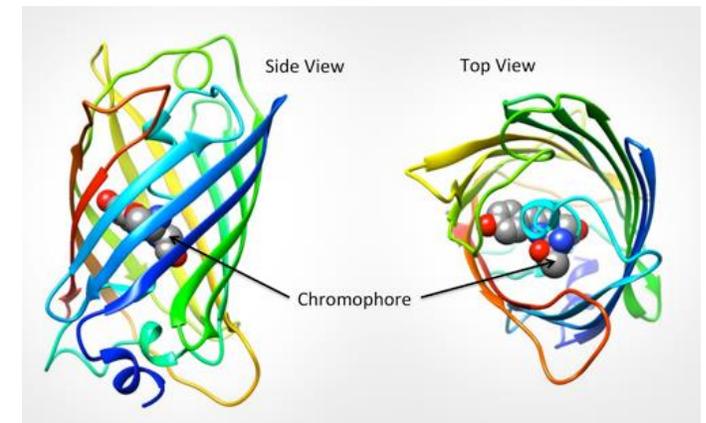





Transgene mice

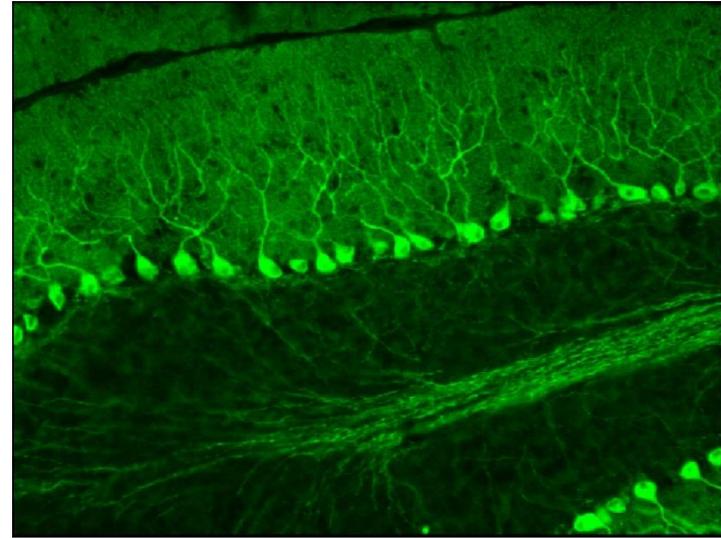

Purkinje cells

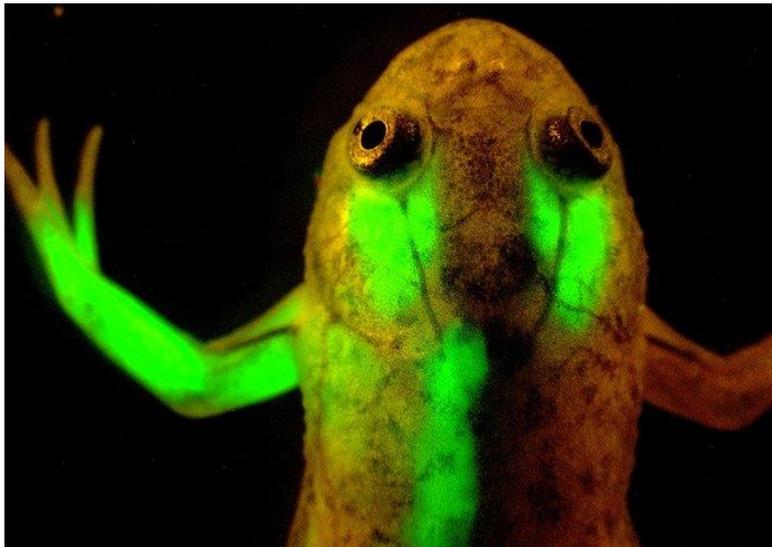

Frog muscle cells

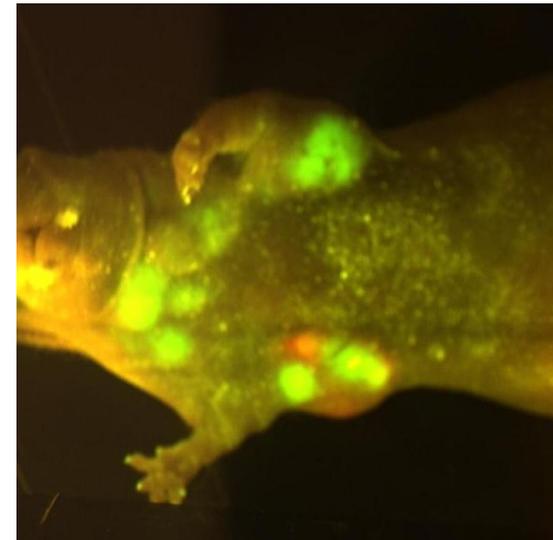

Tumor cells

2008. Nobel prize in chemistry

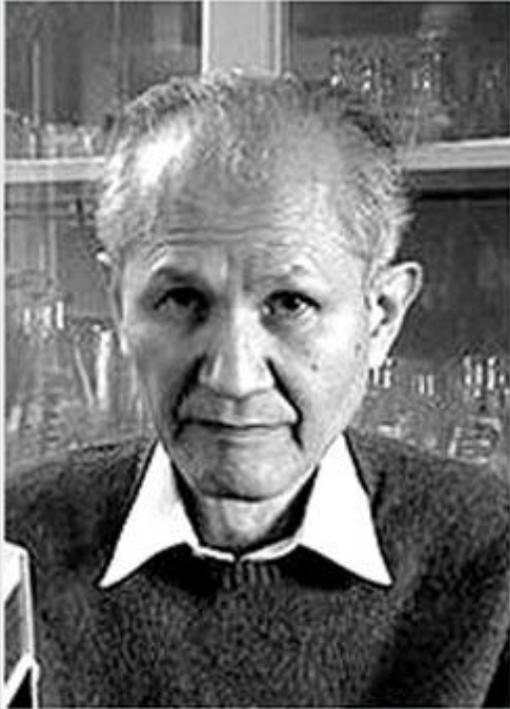


Photo: J.
Henriksson/SCANPIX

Osamu Shimomura



Photo: J.
Henriksson/SCANPIX

Martin Chalfie



Photo: UCSD

Roger Y. Tsien

General properties of lasers

light **a**mplification by **s**timulated **e**mission of **r**adiation




- monochromatic
- coherent
- polarized
- parallel, collimated beam

Possibility of very short pulses – *ps*, *fs*

Possibility of high power – *kW* - *GW*



Penetration of light into the skin

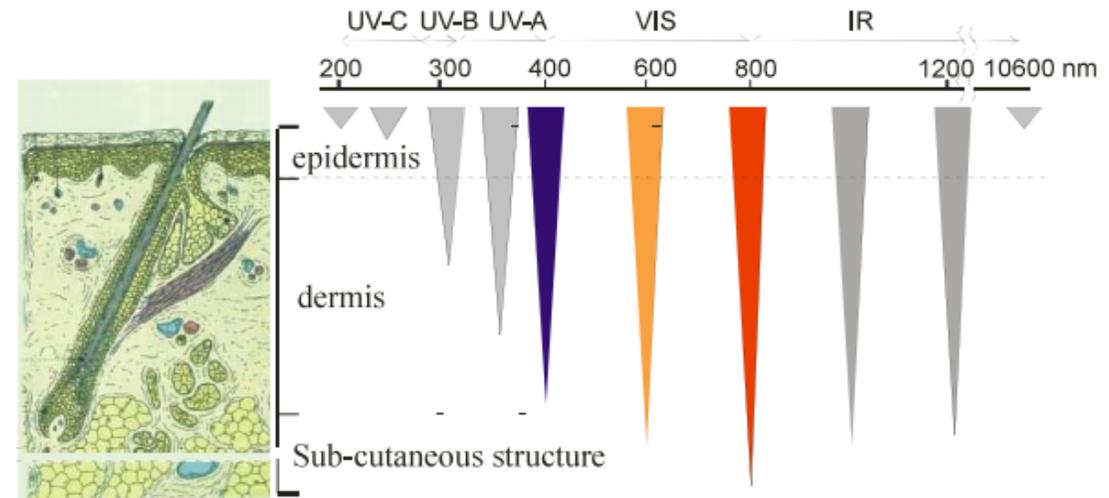



Light intensity is attenuated due to absorption, reflection, refraction.

Penetration depth depends on the wavelength.

Confocal laser scanning microscope

Confocal concept: a focused laser beam is used to produce a small spot illumination on the specimen, and a pinhole in front of the detector eliminates out-of-focus signal


- laser beam – focused illumination
- excitation filter – selected wavelength
- point-by-point scanning
- motorized XY scanning
- „optical sectioning”
- 3D imaging

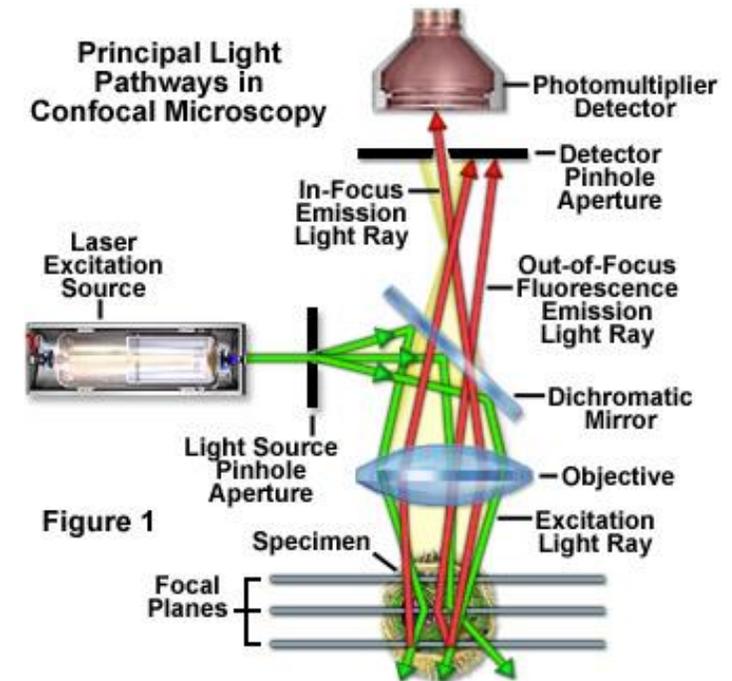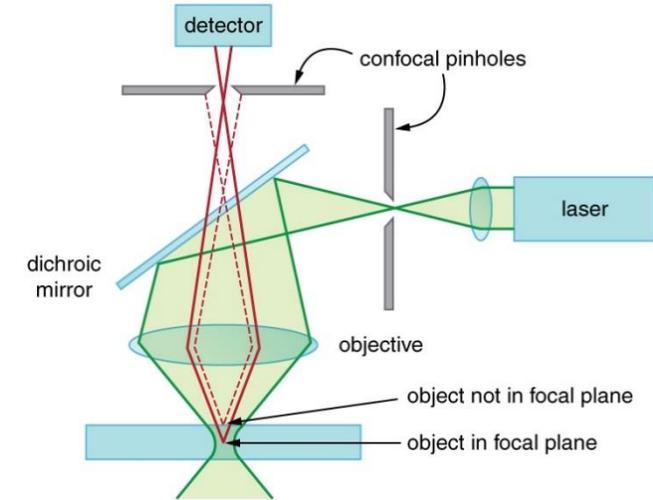


Comparison the imaging of fluorescence and confocal microscopes

Confocal and Widefield Fluorescence Microscopy


fluorescence

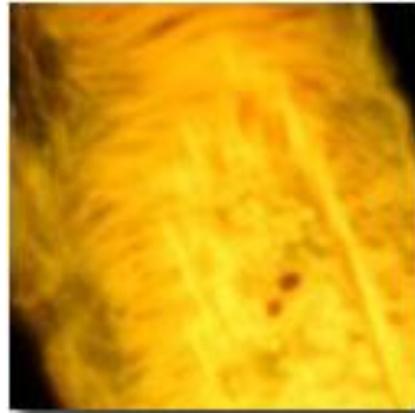

(a)

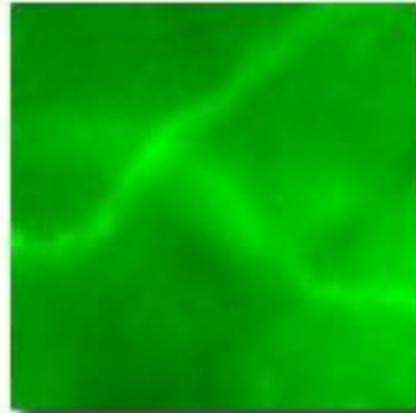


(b)

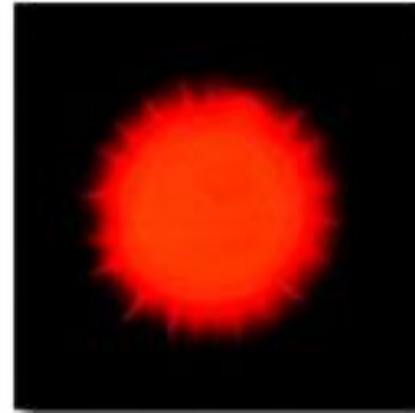


(c)


confocal

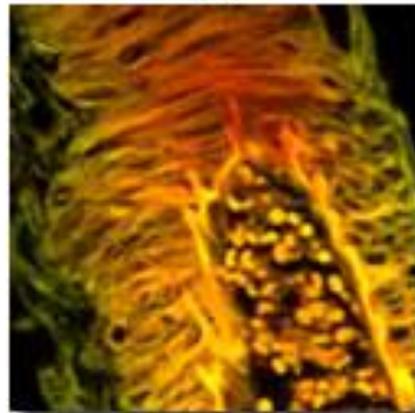

(d)

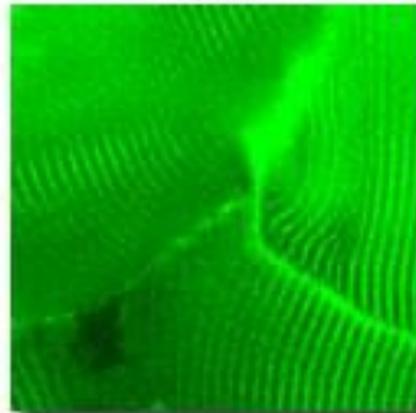

(e)

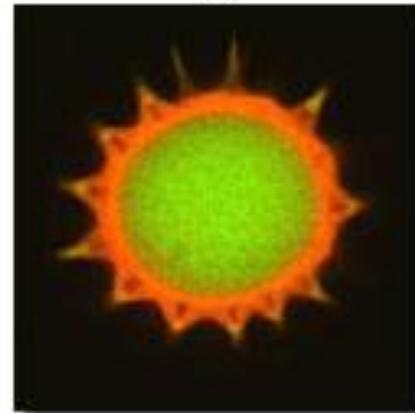

(f)

Figure 1

human medulla

rabbit muscle

pollen

Two-photon microscopy



- 1931. Maria Göppert-Mayer
- in the excited molecule two photon absorb simultaneously
- femtosecond laser source ~ high flux of excitation photons
- 1990. first two-photon excitation microscope
- Wiefried Denk, Cornell University



Maria Göppert-Mayer (1906-1972)




Wiefried Denk (1957-)

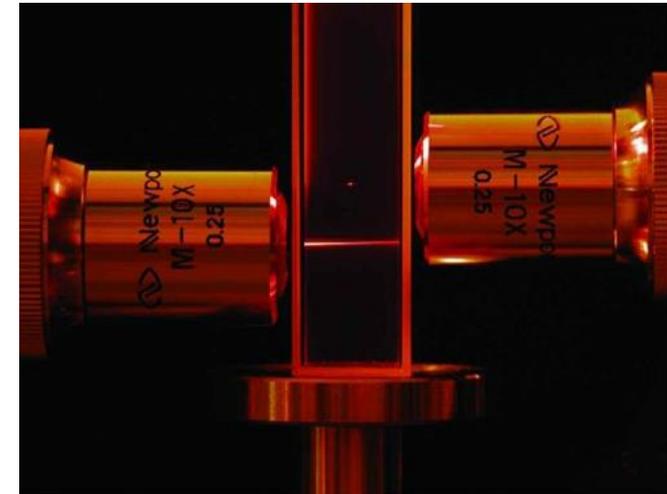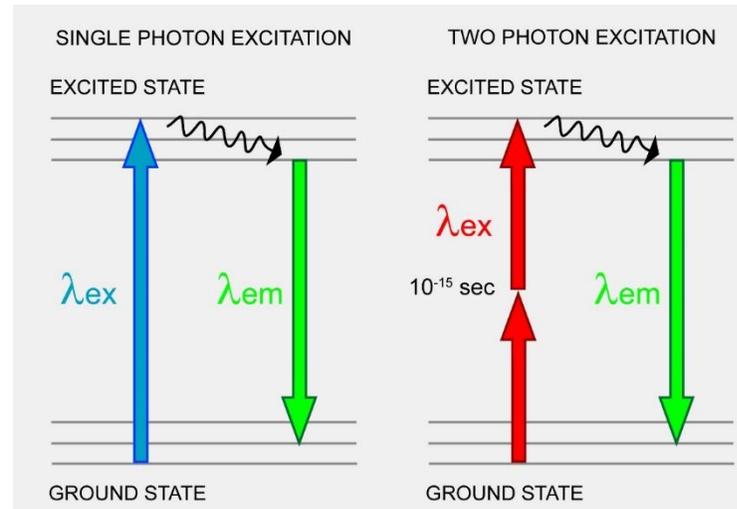


Light absorption and emission spectrum

One photon excitation

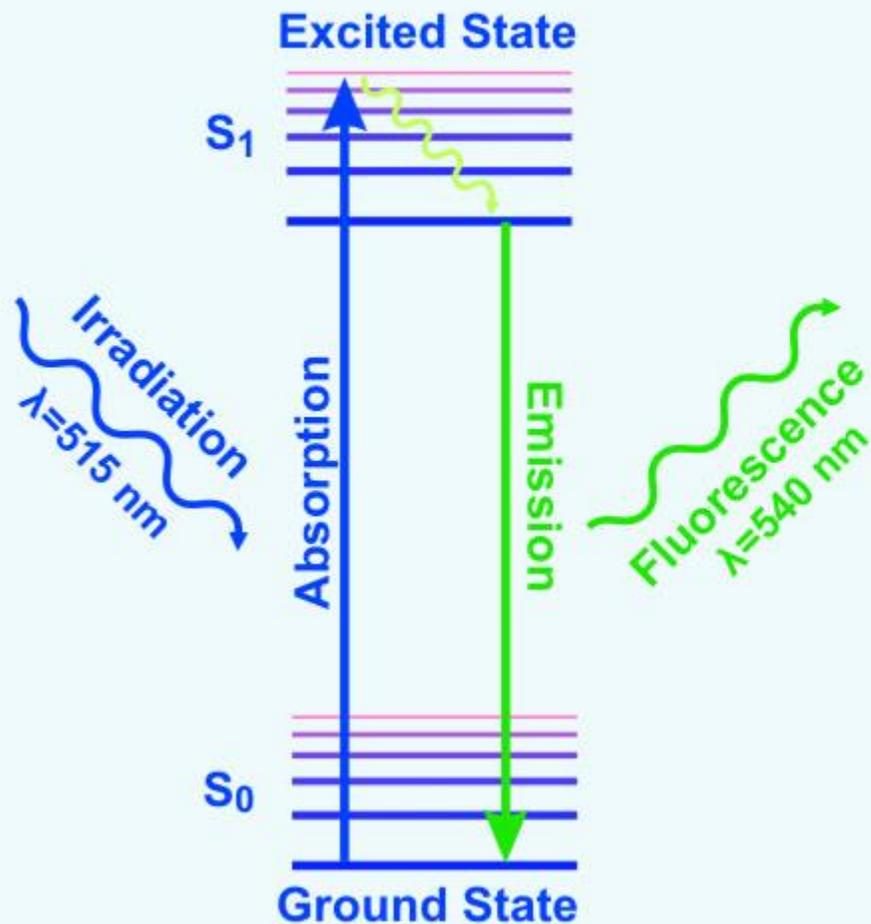


Two photon excitation

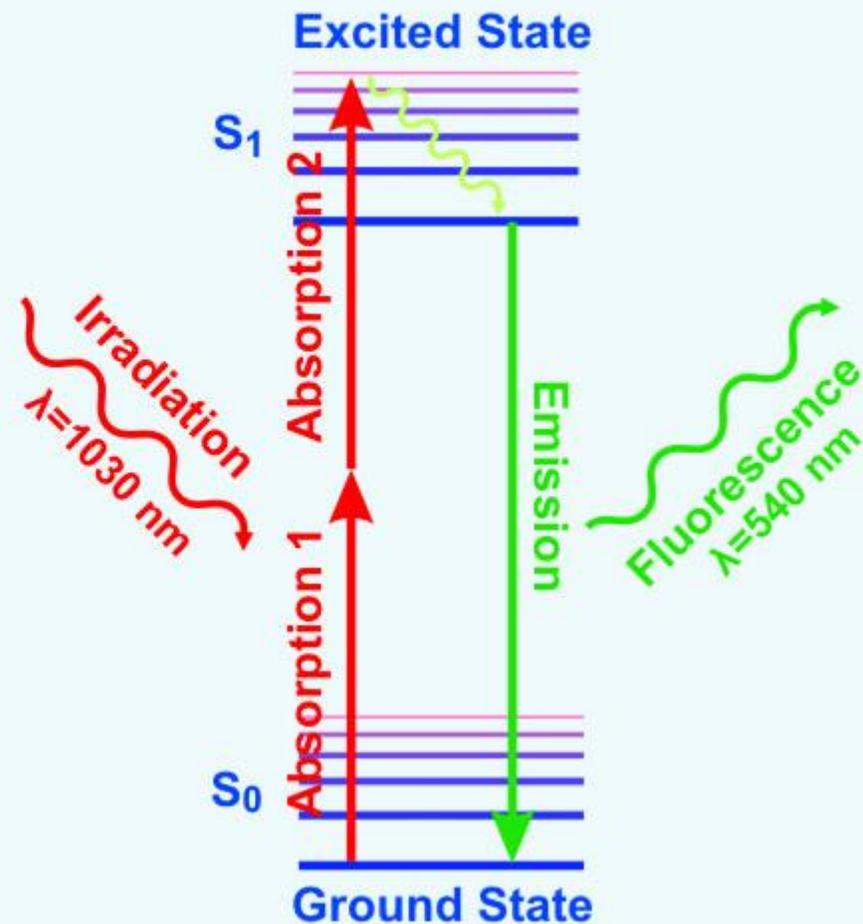


Advantages


- excitation only in a tiny focal volume – reject out-of-focus
- low laser power – *in vivo* imaging
- tunable laser source – infrared spectral range (700-1300 nm) – reduced scattering
- deep penetration
- effective signal detection
- optical sectioning – 3D imaging
- imaging without labeling

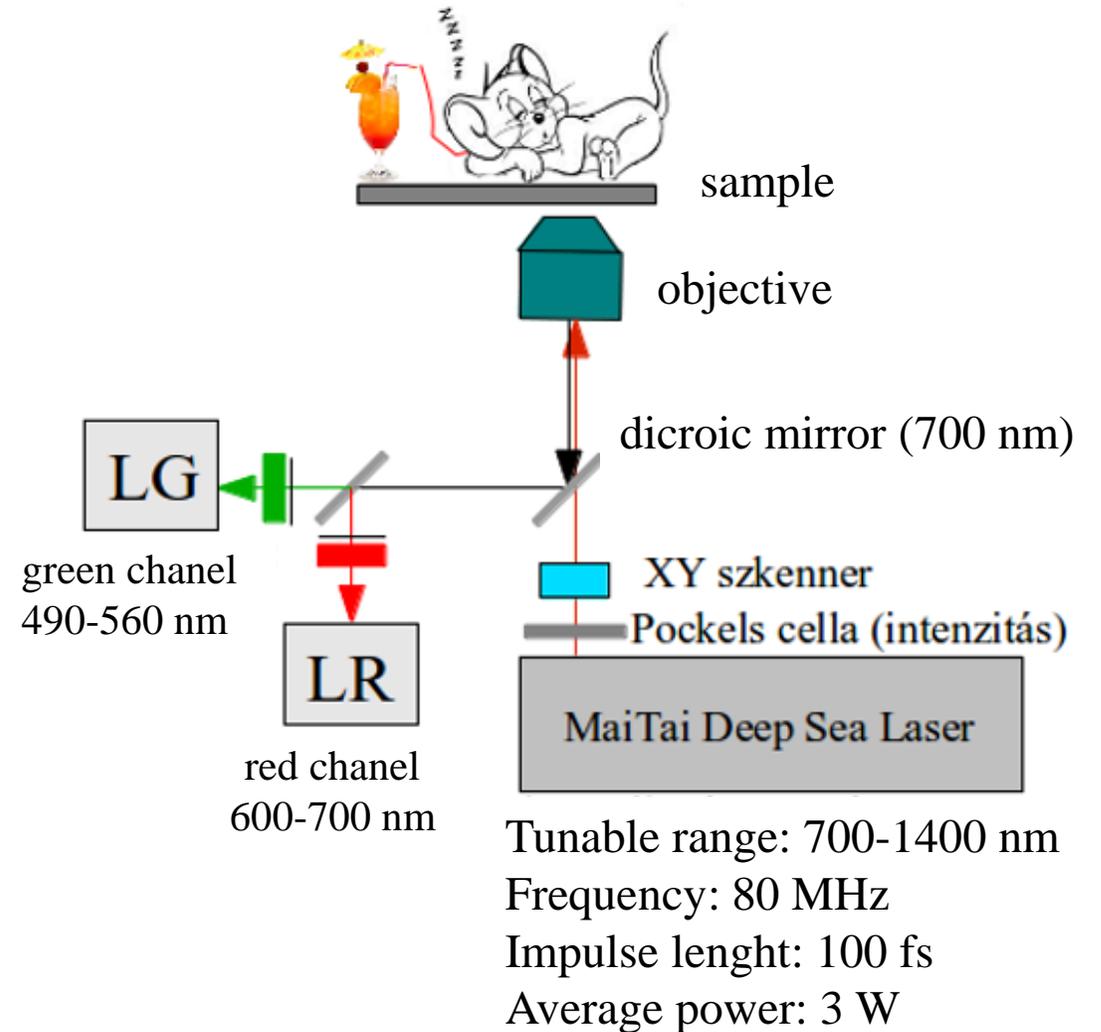


Label-free imaging

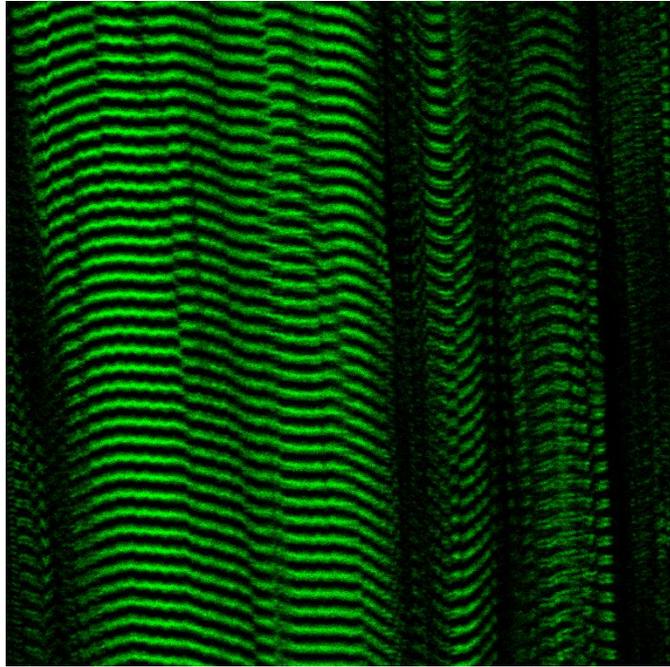


myosin

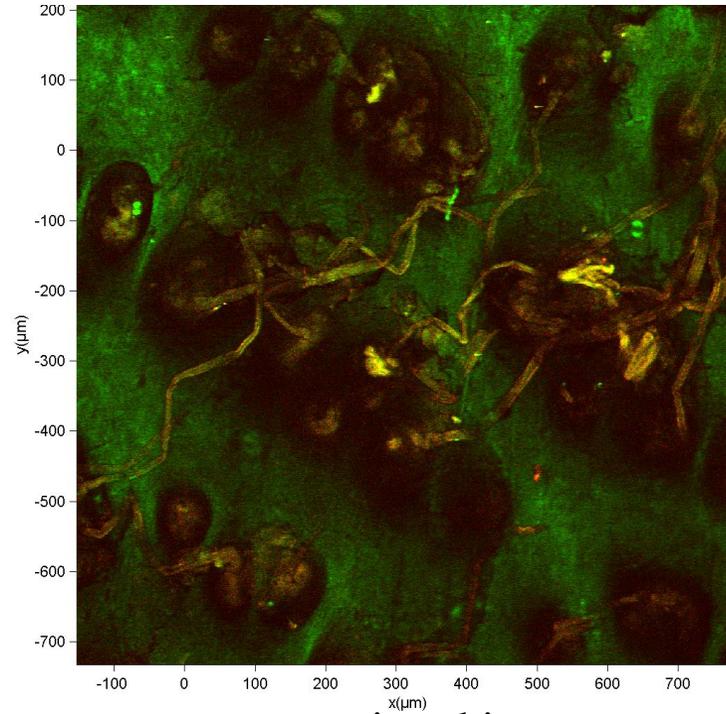

mice skin

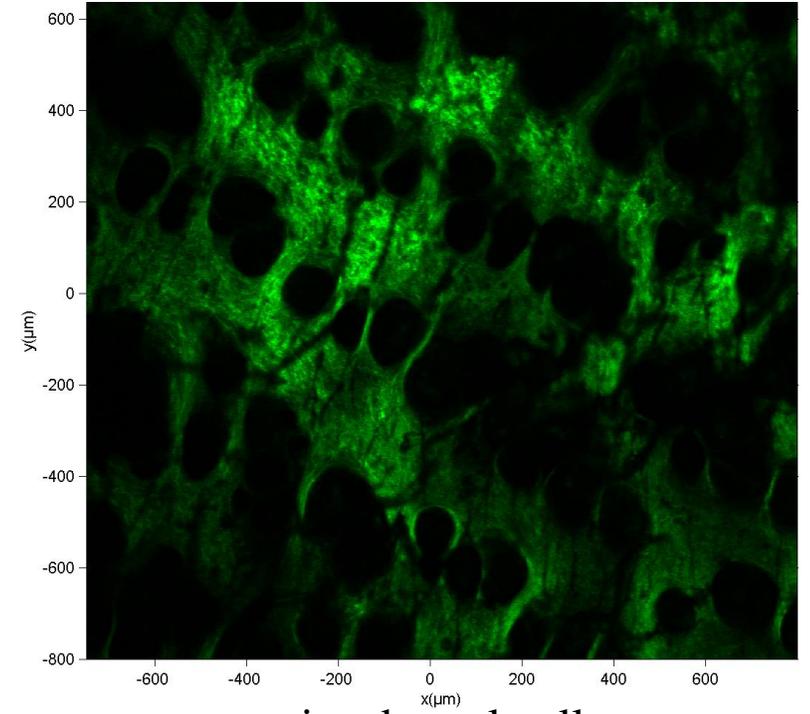


mice dermal collagen

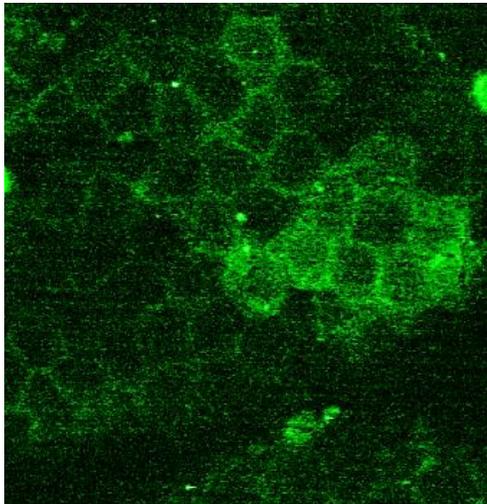


mice skin - keratin



myelin sheaths

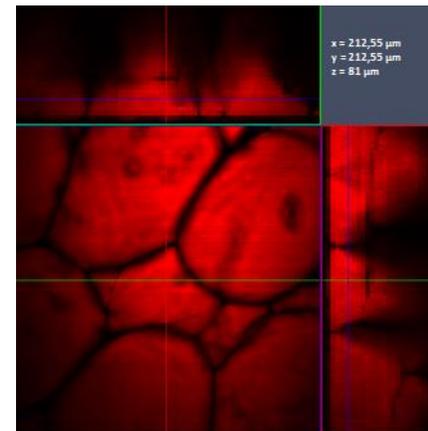



adipocytes

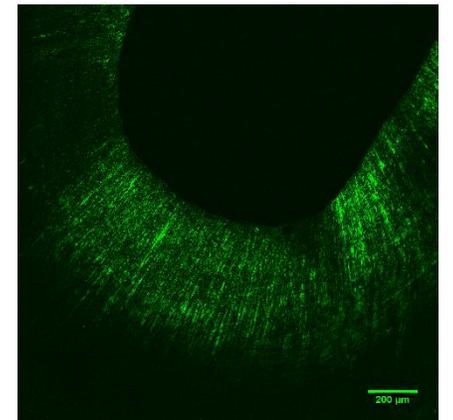

dental tubules


3D imaging

Comparison the dermal collagen structure of a control and type 2 diabetes affected mice

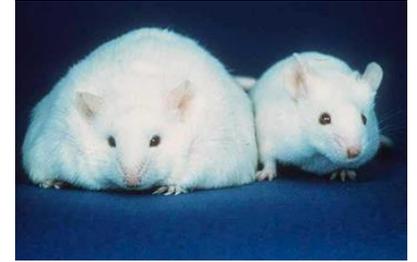


Optical sectioning,
 $z = 80 \mu\text{m}$
 $200 \mu\text{m} \times 200 \mu\text{m}$
exc: 990 nm

Multiple fluorescent labeling

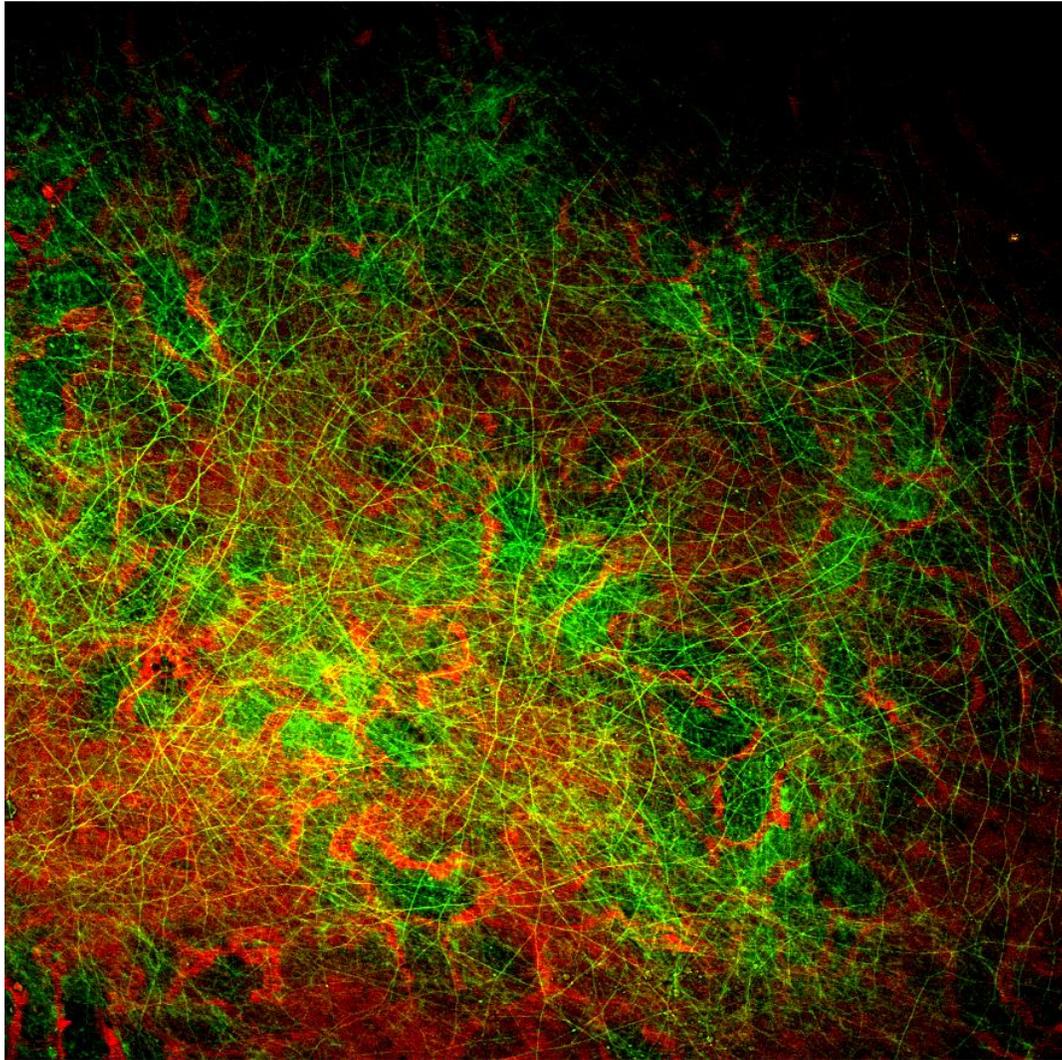


renal cortex

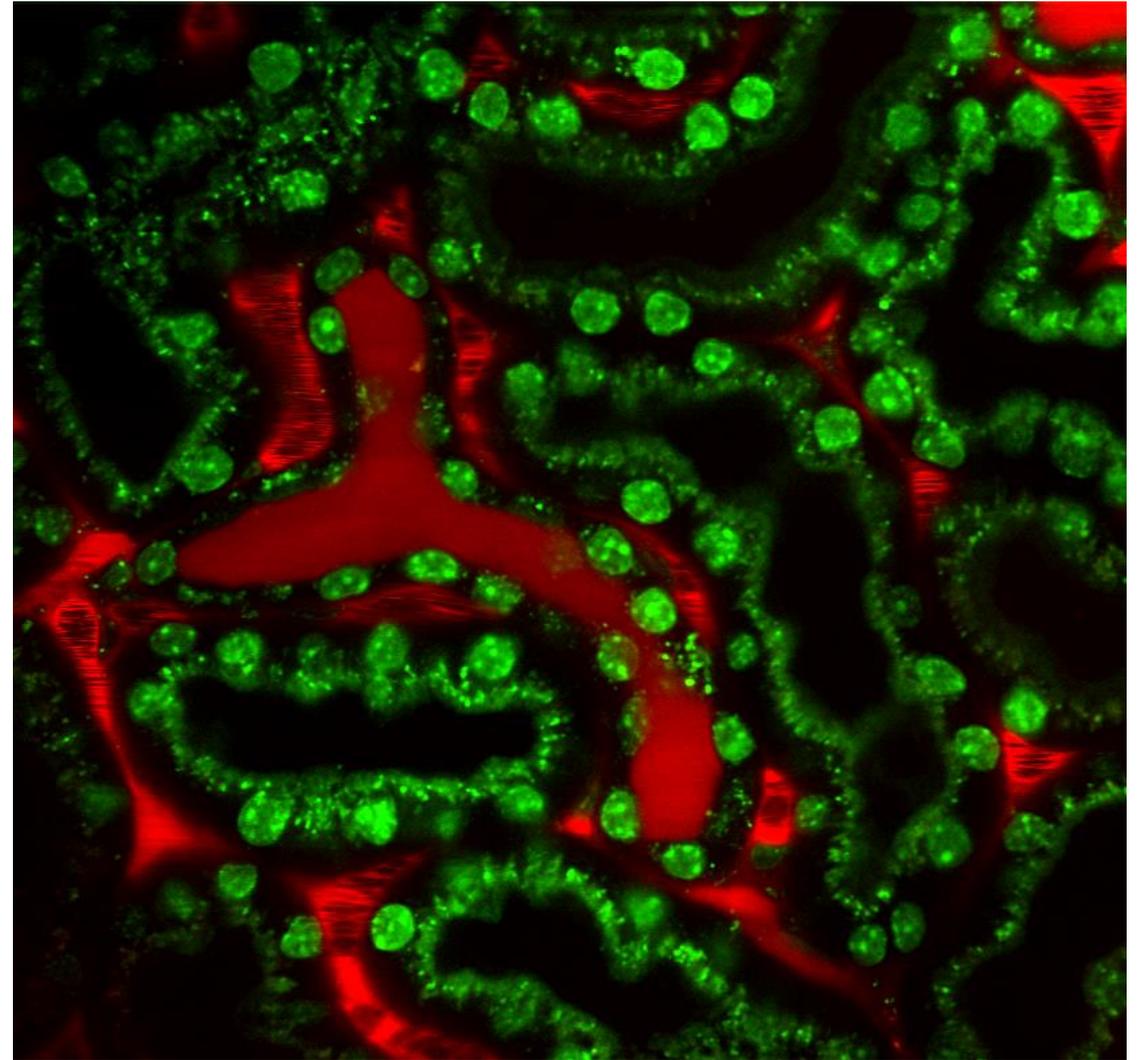


collecting ducts and JGA cells

green: quinacrine (renin-positive granules), Hoechst 33342 (nuclei), and autofluorescence; **red:** 70 kDa rhodamine dextran (vasculature).

How big are things?

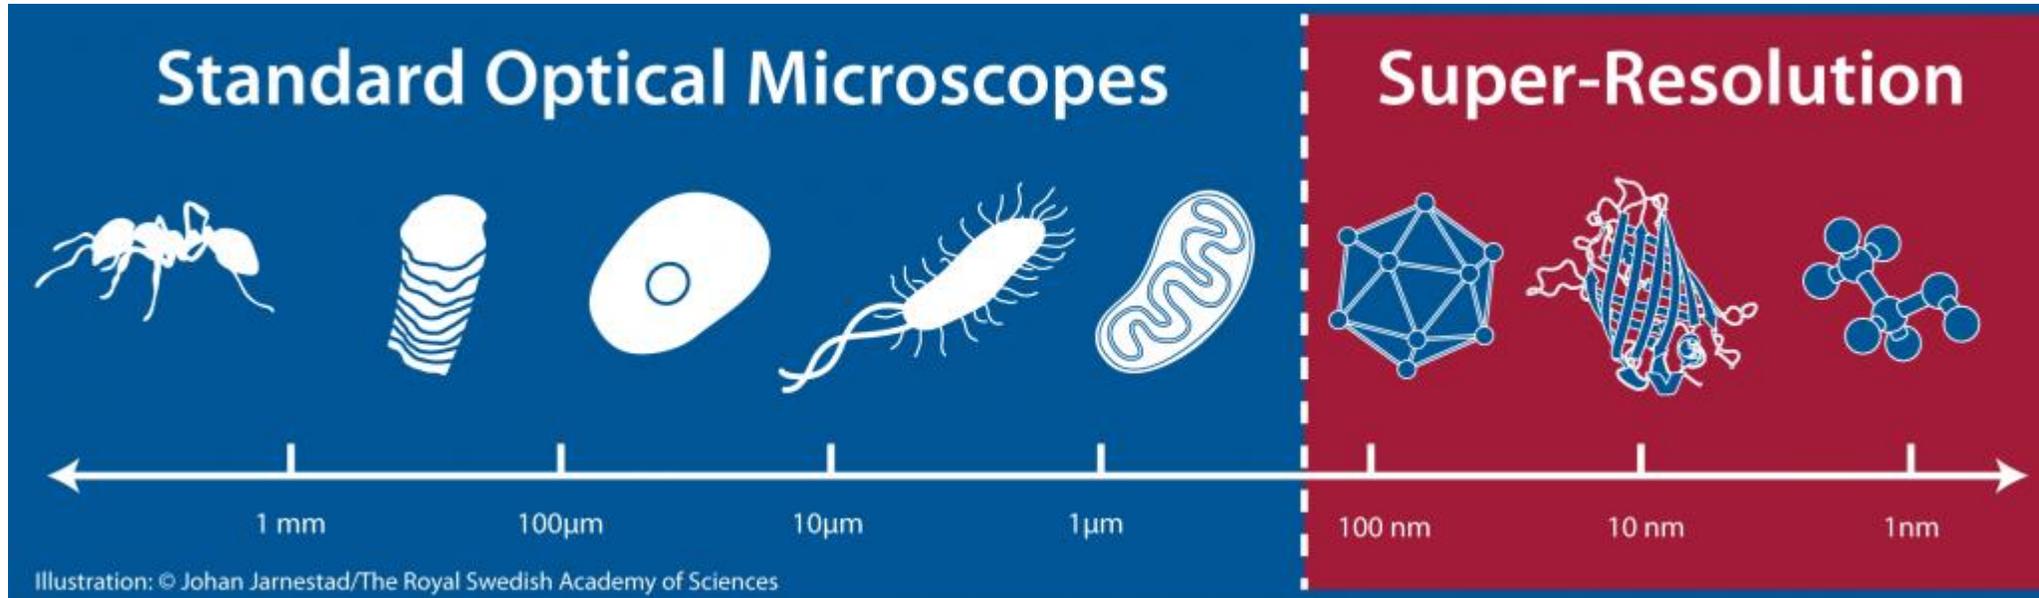


Superresolution microscopy



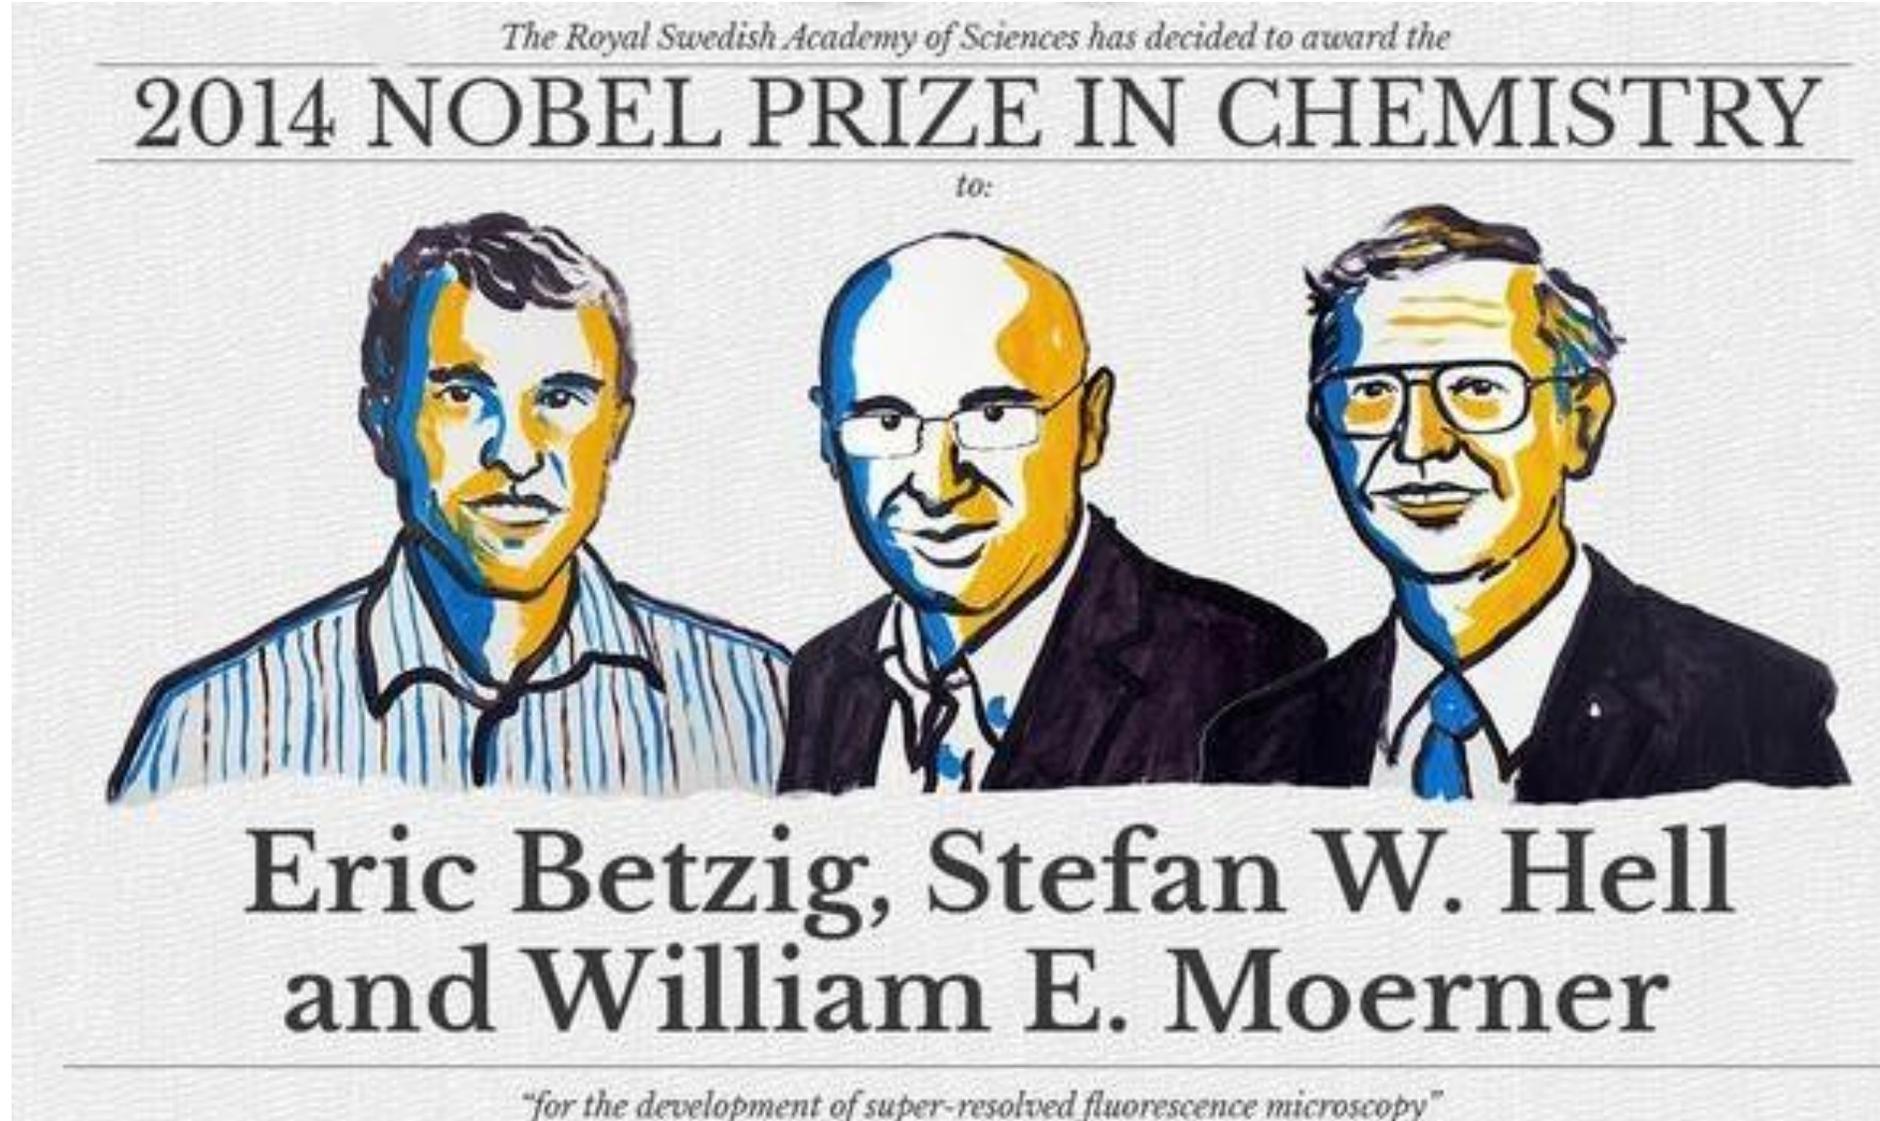


Superresolution microscope

- 2014. Eric Betzig, Stefan W. Hell és William E. Moerner were awarded Nobel-prize in chemistry
- STED: stimulated emission depletion microscopy
- 2018. August – STED device arrived in our Institute
- allows for images to be taken at resolutions below the diffraction limit

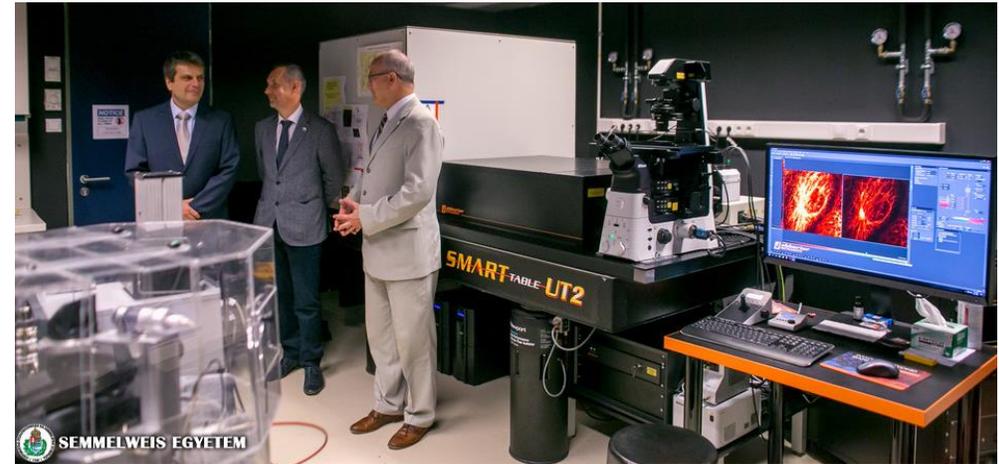


- excitation laser + depletion laser
- point-by-point scanning
- STED (stimulated emission depletion microscopy)

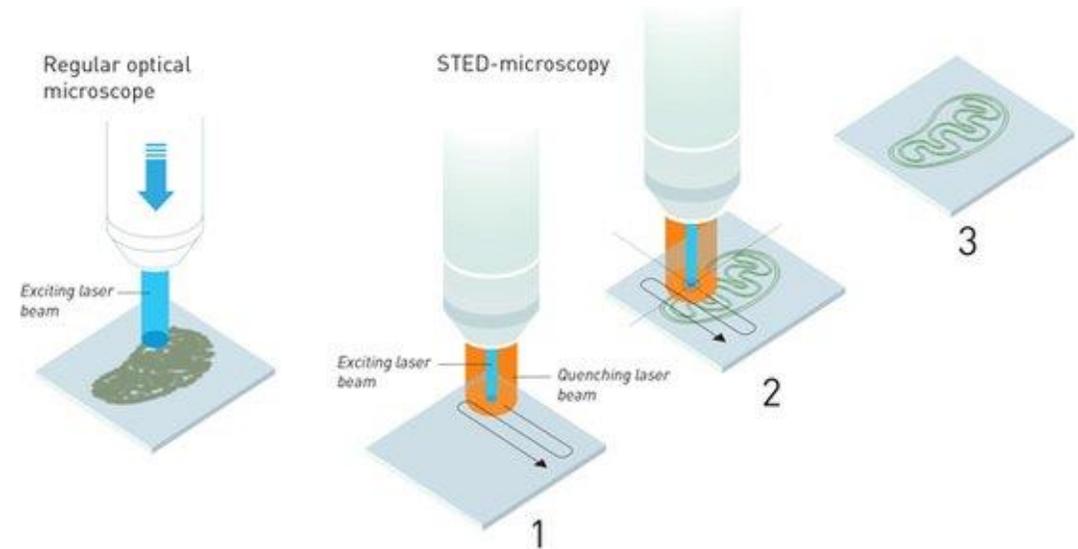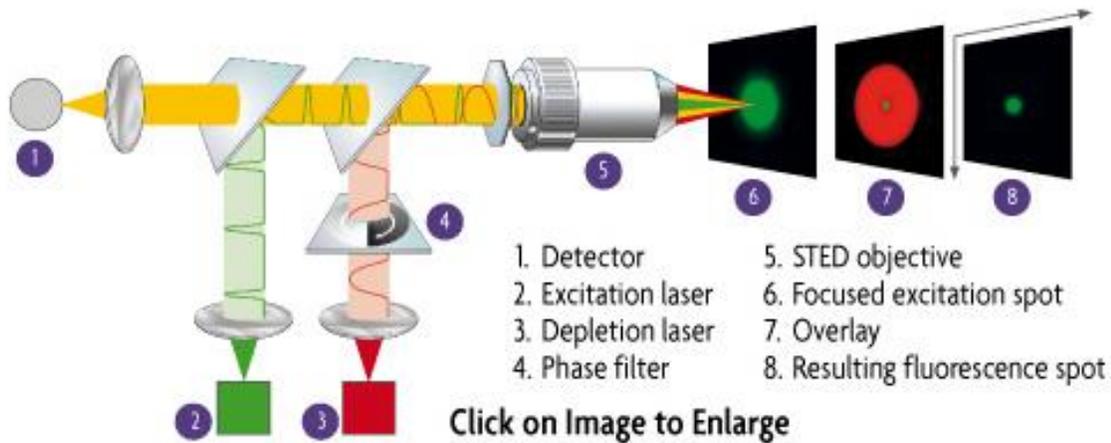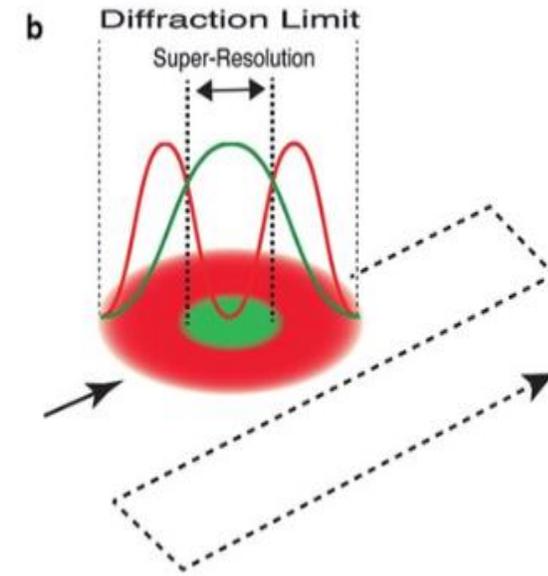


confocal


STED

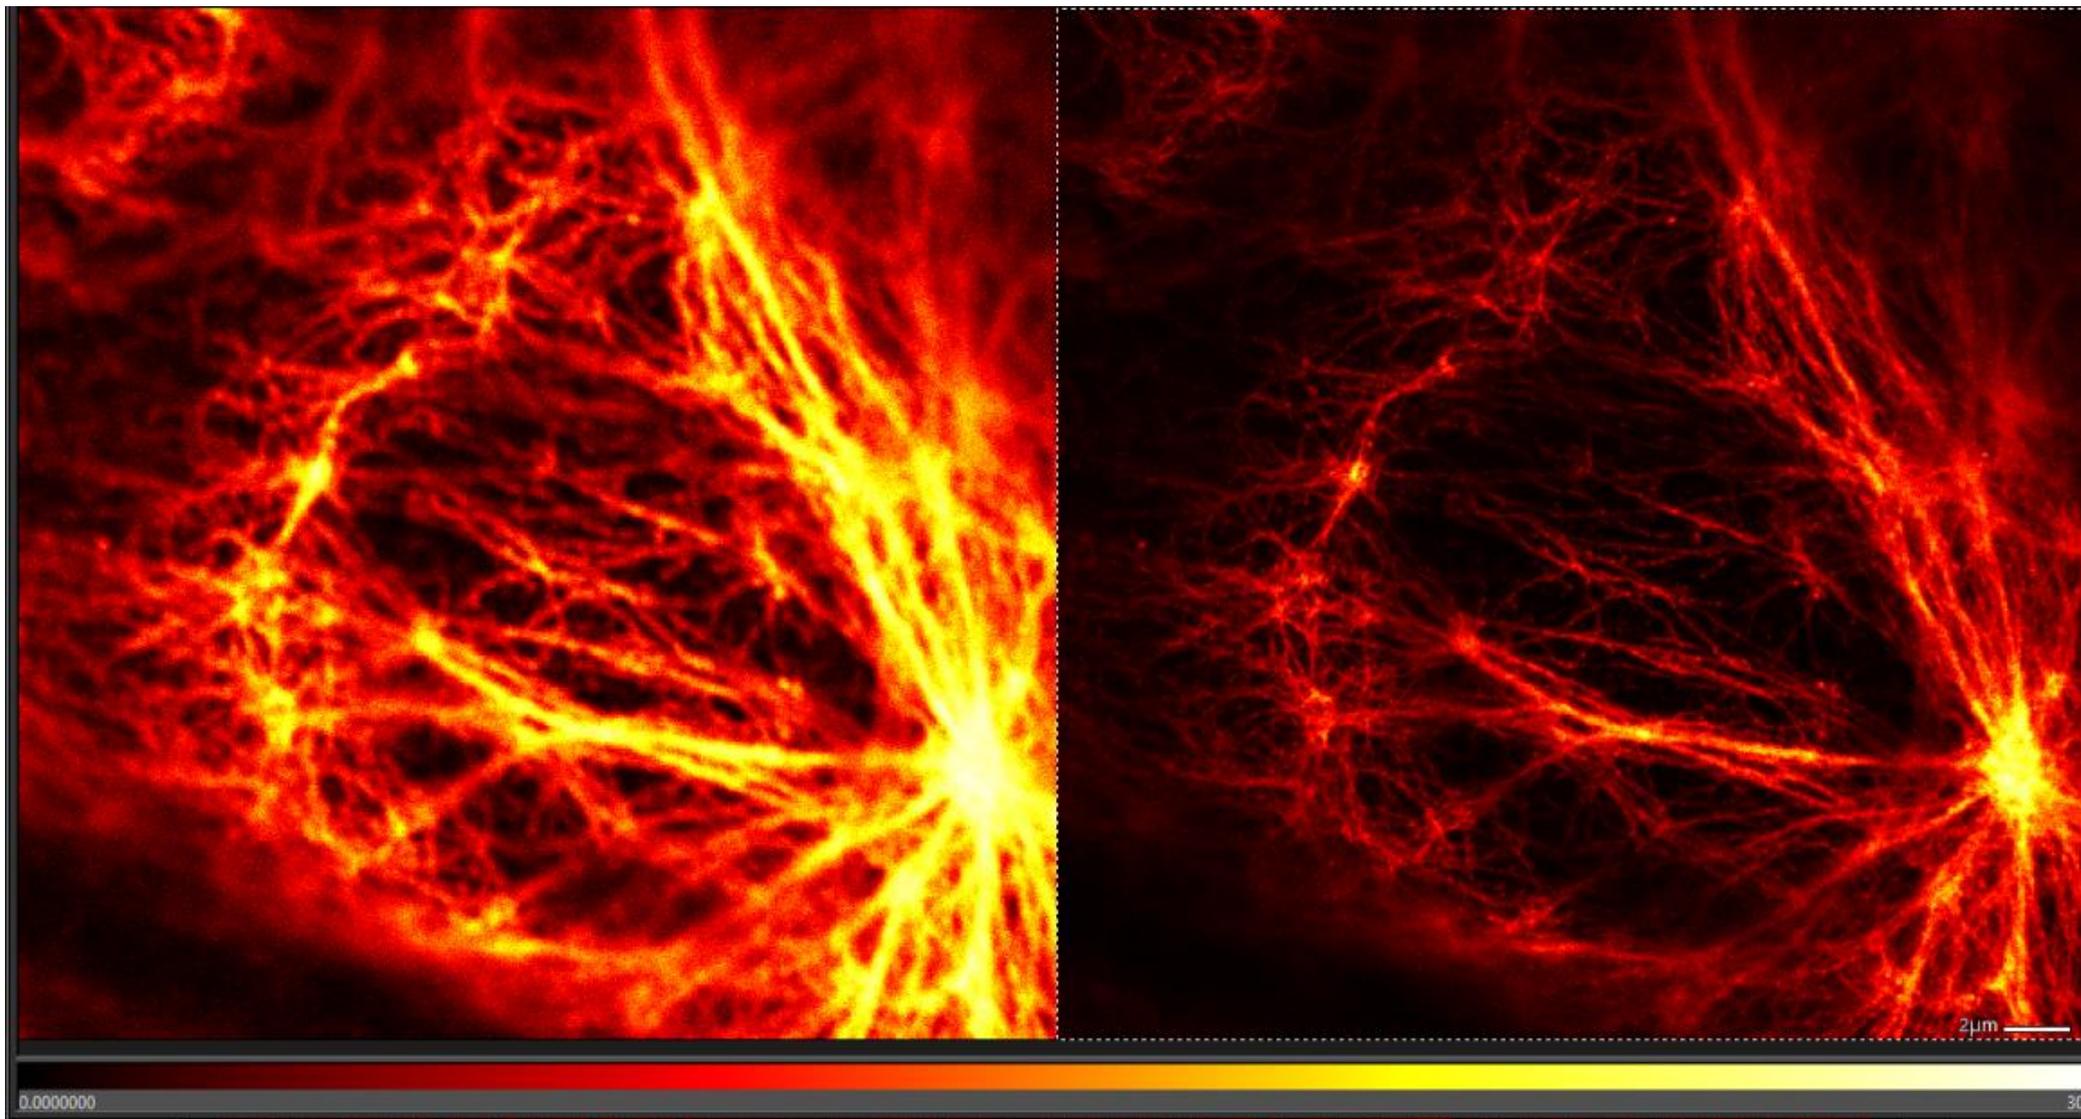

confocal

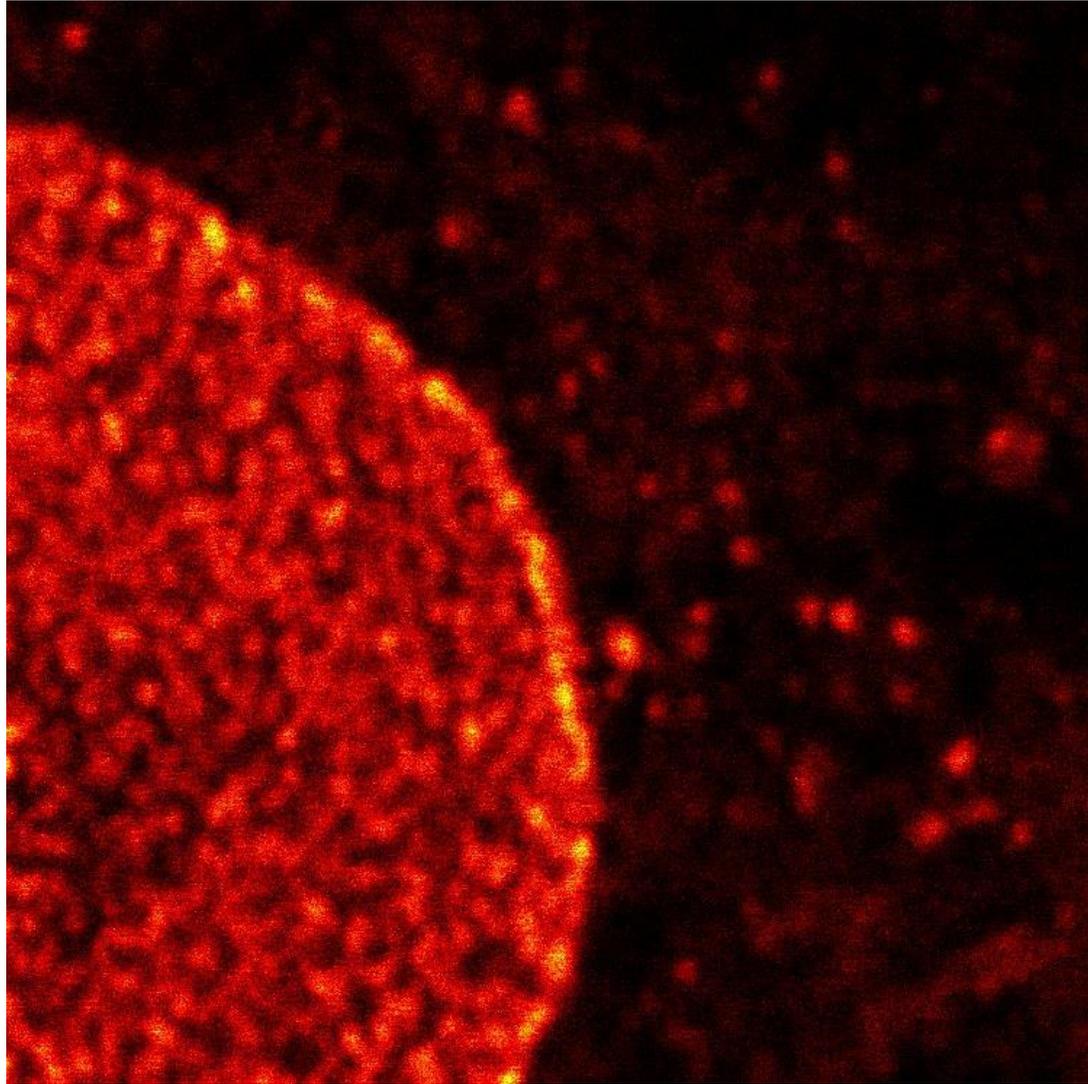

STED

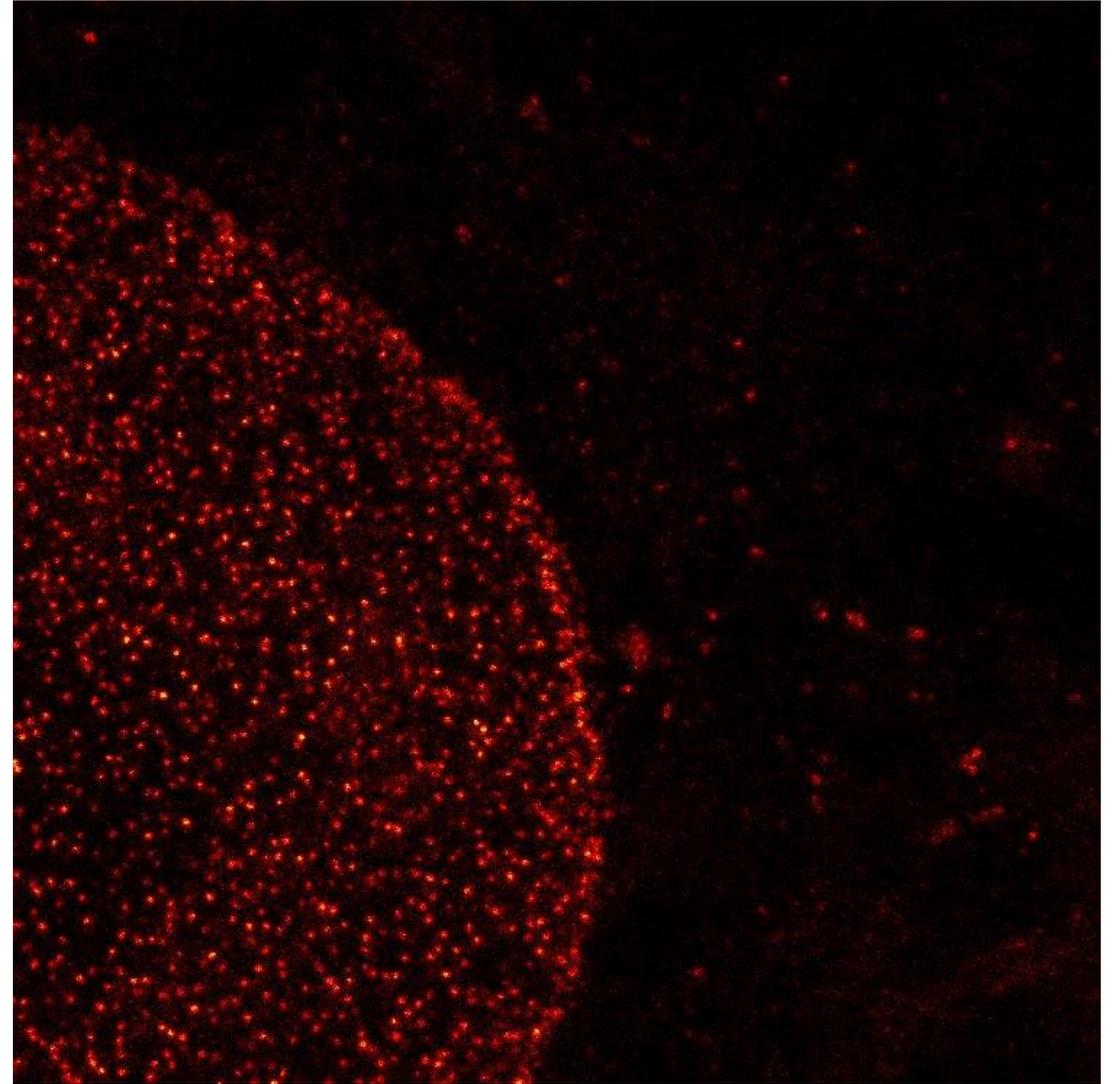

Checklist

✓ resolution limit of image formation

✓ Abbe's principle

$$\delta = 0,61 \frac{\lambda}{n \sin \omega}$$

✓ working principle of fluorescence microscope: illumination, excitation/emission spectra, Stokes-shift, function of dichroic mirror

✓ sources of fluorescence: intrinsic, extrinsic



✓ GFP protein

✓ working principle of confocal microscope: illumination, function of pinhole

✓ working principle of two-photon microscope: properties of laser source, excitation/emission spectra, penetration ability, advantages

✓ superresolution microscopy: principle of STED imaging

